

Area Percent Report



Agilent Technologies

Data file: E:\HPLC\data\TEST\0CJK-2 10-28 16-40-44\007-P2-C7-14543917-40-45.D
Sample name: 145439
Instrument: 2DLC
Acq. method: F0.6 285nm.M
Analysis method: F0.6 285nm.M
Sample type: Sample
Location: P2-C7
Injection: 1 of 1
Injection volume: 0.500


FLOW RATE : 0.6ml/min
COLUMN : ACE C18 50*2.1 2um

COLUMN TEMPERATURE : 30

GRADIENT PROGRAM :

TIME(MIN) MOBILE PHASE-A(H₂O+0.1TFA) MOBILE PHASE-B(CH₃CN+0.1TFA)

0	90%	10%
6	0%	100%
8	0%	100%

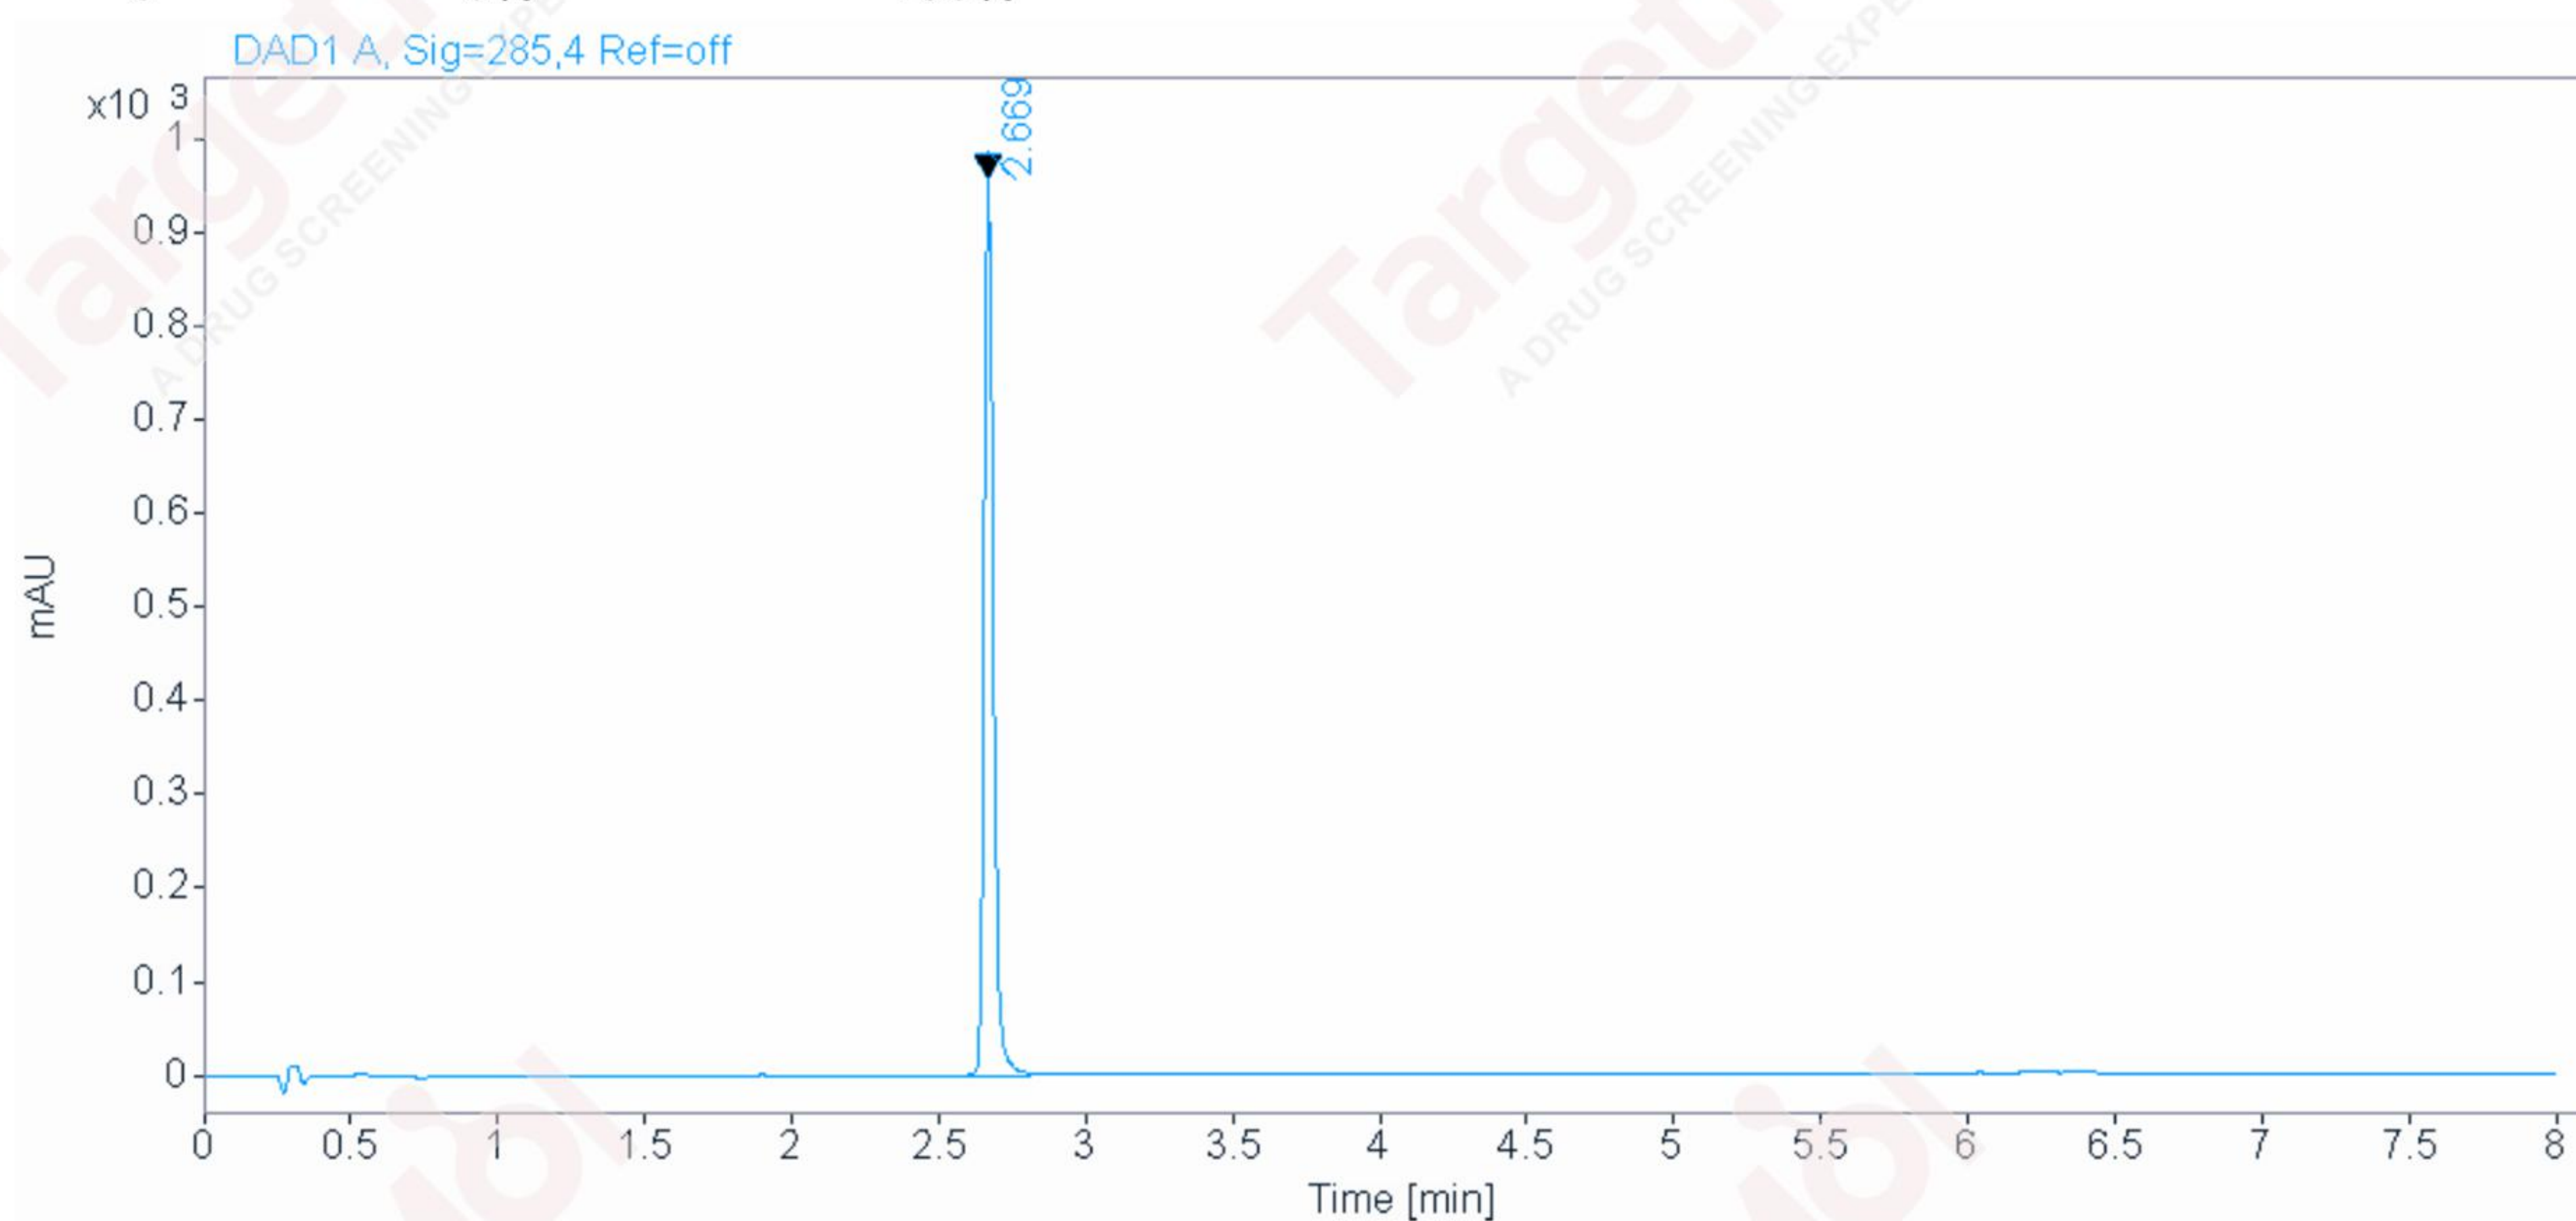

Signal: DAD1 A, Sig=285,4 Ref=off

RT [min]	Type	Width [min]	Area	Height	Area%	Name
2.669	BB	0.0359	2128.7493	957.6265	100.0000	
	Sum		2128.7493			