

Analysis: XHDa-re-1

Path: Home/YL Research

Based on method: Triplets Method

Created	07-Jun-2019 21:32:07	visionCATSuser
Modified	07-Jun-2019 23:23:11	visionCATSuser
Last HPTLC log	07-Jun-2019 23:23:11	Analysis modified
Explorer notes		

Track	Vial ID	Description	Volume	Position	Type
1	MeOH blank	MeOH Blank	2.0 µl	A1	Sample
2	Mixture 100	Mixture 500ng	5.0 µl	A2	Sample
3	9-THC 100	D9-THC 500ng	5.0 µl	A3	Reference
4	CBD 100	CBD 500ng	5.0 µl	A4	Reference
5	CBN 100	CBN 500ng	5.0 µl	A5	Reference
6	CBG 100	CBG 500ng	5.0 µl	A6	Reference
7	CBC 100	CBC 500ng	5.0 µl	A7	Reference
8	THCV 100	THCV 500ng	5.0 µl	A8	Reference
9	CBDV 100	CBDV 500ng	5.0 µl	A9	Reference
10	8-THC 100	D8-THC 500ng	5.0 µl	A10	Reference
11	THCA-A 100	THCA-A 500ng	5.0 µl	A11	Reference
12	CBDA 100	CBDA 500ng	5.0 µl	B1	Reference
13	CBGA 100	CBGA 500ng	5.0 µl	B2	Reference
14	Mixture 100	Mixture 500ng	5.0 µl	A2	Sample
15	MeOH blank	MeOH Blank	2.0 µl	A1	Sample

Sequence table notes

A track marked with ⚠ means: the application type is overridden in some evaluation(s).

System setup:

Software	Server User-PC, version 2.5.18072.1
ATS4	S/N:080713
Chamber	N/A
Derivatization dip	N/A
Scanner3	S/N:031025
Visualizer	S/N:230515

Chromatography

Plate layout:

Stationary phase	Merck, HPTLC plates silica gel 60 F 254
Plate format	200.0 x 100.0 mm
Application type	User
Application	Position Y: 10.0 mm, length: 8.0 mm, width: 0.0 mm
Track	First position X: 20.0 mm, distance: 11.4 mm
Solvent front position	70.0 mm
Notes	

Take image clean plate 1a - Visualizer (S/N: 230515):

XHDa-re-1

visionCATS

Quality	Enhanced
RT White	auto capture, Auto, level 85 %, Band
R 254	auto capture, Auto, level 85 %, Band
Instrument diagnostics	Valid diagnostics
Documentation step label	
Notes	

Application 1 - ATS 4 (S/N: 080713):

Spray gas	NI
Sample solvent type	Methanol
Filling speed	15 µl/s
Predosage volume	200 nl
Retraction volume	200 nl
Dosage speed	150 nl/s
Filling quality	User
Rinsing cycles / vacuum	1 / 4 s
Filling cycles / vacuum	1 / 4 s
Rinsing solvent name	Methanol
Nozzle temperature	Unheated
Rack in use	Standard
Instrument diagnostics	Valid diagnostics
Notes	

Development 1 - Chamber:

Tank	TTC 20x10
Mobile phase	
Saturation time	20 min
Use saturation pad	true
Use smartALERT	false
Volume front through	10 ml
Volume rear through	20 ml
Drying time	5 min
Drying temperature	Room temperature
Notes	

Take image developed plate 1a - Visualizer (S/N: 230515):

Quality	Enhanced
RT White	auto capture, Auto, level 85 %, Band
R 254	auto capture, Auto, level 85 %, Band
R 366	auto capture, Auto, level 85 %, Band
Instrument diagnostics	Valid diagnostics
Documentation step label	
Notes	

Scan developed plate 1b - Scanner 3 (S/N: 031025):

XHDa-re-1

visionCATS

Scanner type	Single λ
Optimization for	Resolution
Measurement mode	Absorption
Filter	n/a
Detector mode	Automatic
Scanning speed	20 mm/s
Data resolution	100 μ m/step
Slit	5 x 0.2 mm, micro
Partial scan	No
Lamp	Deuterium & Tungsten
Wavelength(s)	254 nm
Instrument diagnostics	Valid diagnostics
Documentation step label	
Notes	

Derivatization 1 - dip:

Reagent name	Fast Blue B salt
Dipping speed	3
Dipping time	5 s
Reagent preparation	1g Fast Blue B salt in 200mL water
Heating	none
Notes	Air dry for 5 minutes

Take image derivatized plate 1a - Visualizer (S/N: 230515):

Quality	Enhanced
RT White	auto capture, Auto, level 85 %, Band
R 366	auto capture, Auto, level 85 %, Band
Instrument diagnostics	Valid diagnostics
Documentation step label	
Notes	

System suitability tests:

SST settings:

SST tracks	
------------	--

Data acquisition

Application 1 - ATS 4 (S/N: 080713):


Executed	07-Jun-2019 21:33:56 visionCATSuser
----------	-------------------------------------

Development 1 - Chamber:

Executed	07-Jun-2019 22:30:59 visionCATSuser
----------	-------------------------------------

Take image developed plate 1a - Visualizer (S/N: 230515):


Executed	07-Jun-2019 22:55:11 visionCATSuser
----------	-------------------------------------

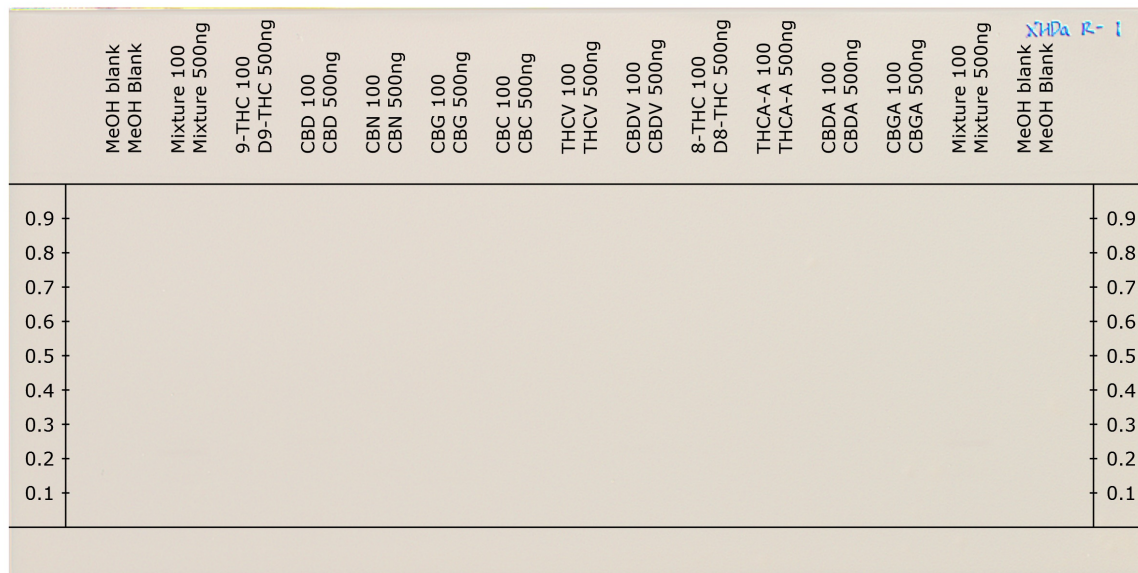

Exposure	0.102 s
Contrast	1
Normalized exposure	Disabled
Clarify	Disabled
White balance	1.00, 1.00, 1.00

R 254


Developed, Remission254

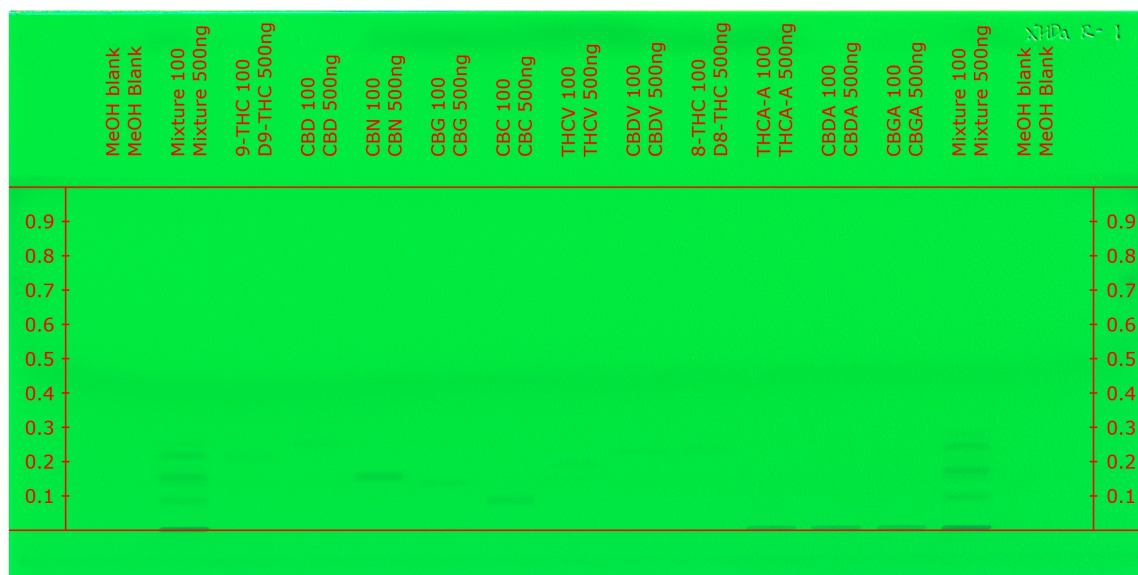

Exposure	0.285 s
Contrast	1
Normalized exposure	Disabled
Clarify	Disabled
White balance	1.00, 1.00, 1.00

XHDa-re-1
R 366

visionCATS
Developed, Remission366

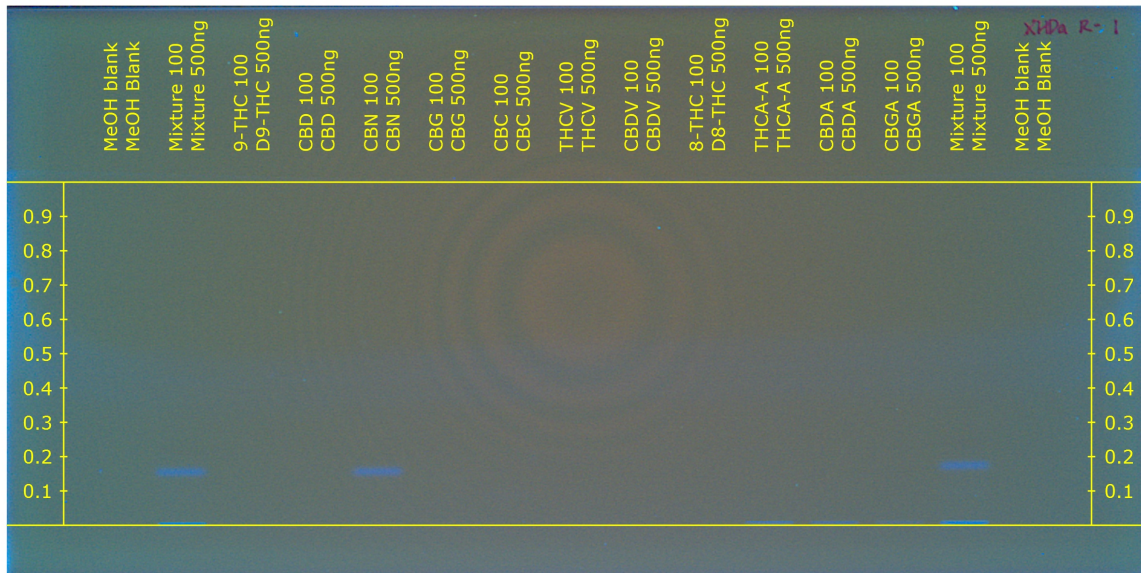

Exposure	9.999 s
Contrast	1
Normalized exposure	Disabled
Clarify	Disabled
White balance	1.00, 1.00, 1.00

Scan developed plate 1b - Scanner 3 (S/N: 031025):


Executed	07-Jun-2019 23:00:26 visionCATSuser
----------	-------------------------------------

Scan:

Wavelength	254 nm
------------	--------

Track 1:

Type	Single λ
------	------------------

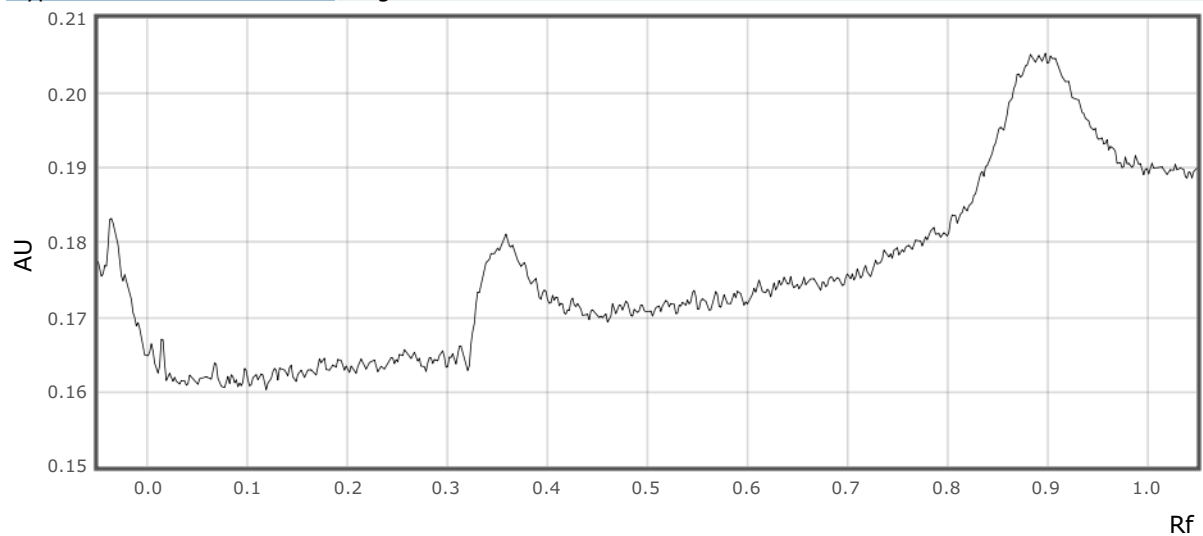


XHDa-re-1

visionCATS


Track 2:

Type Single λ

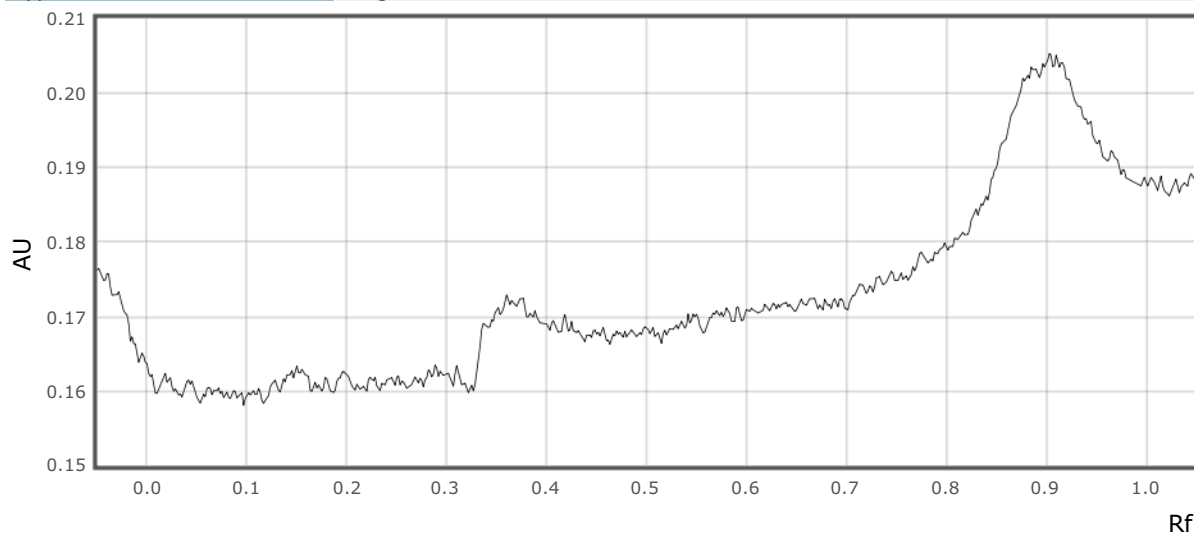


Track 3:

Type Single λ

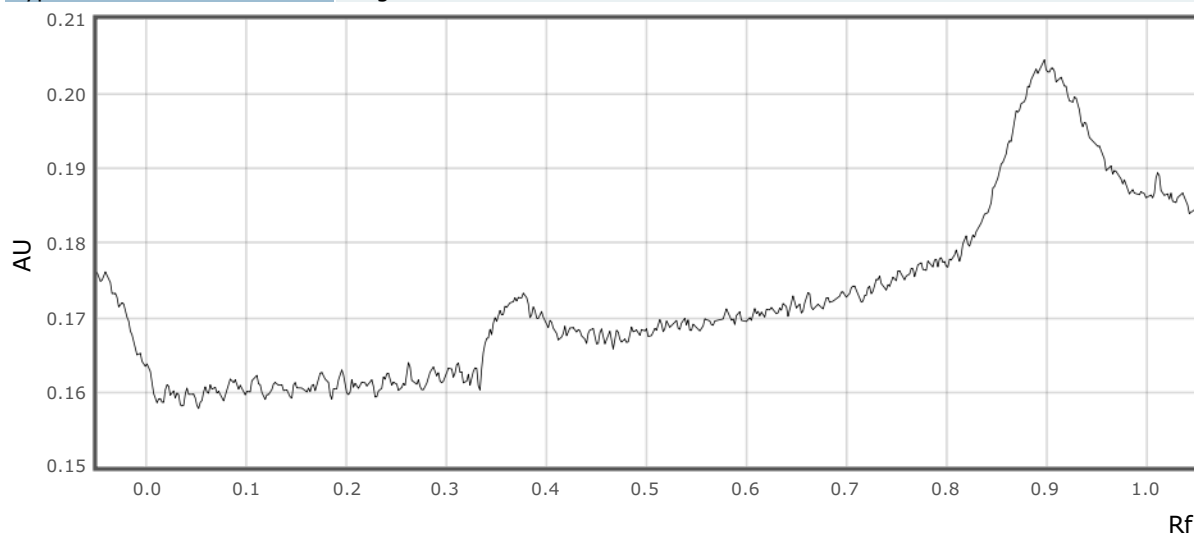


Track 4:

Type Single λ

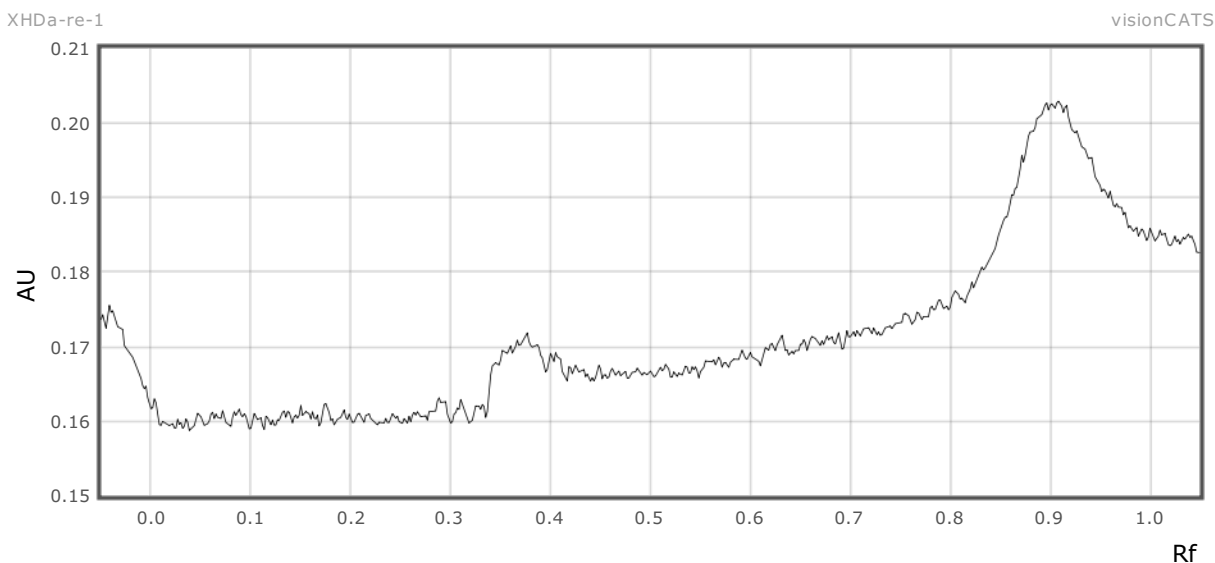


Track 5:

Type Single λ

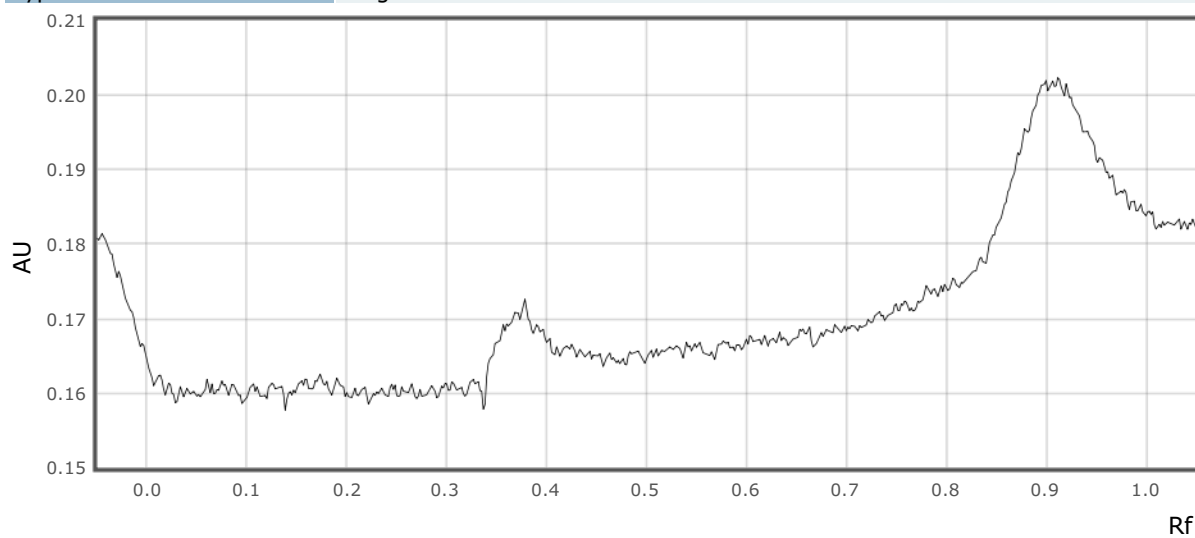


Track 6:

Type Single λ

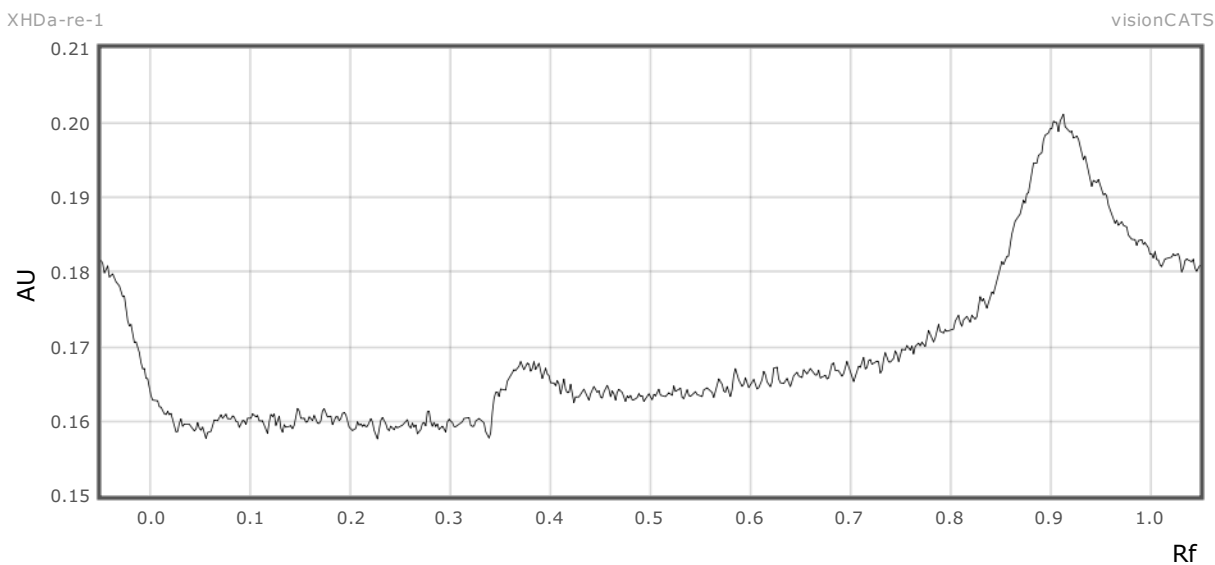


Track 7:

Type Single λ

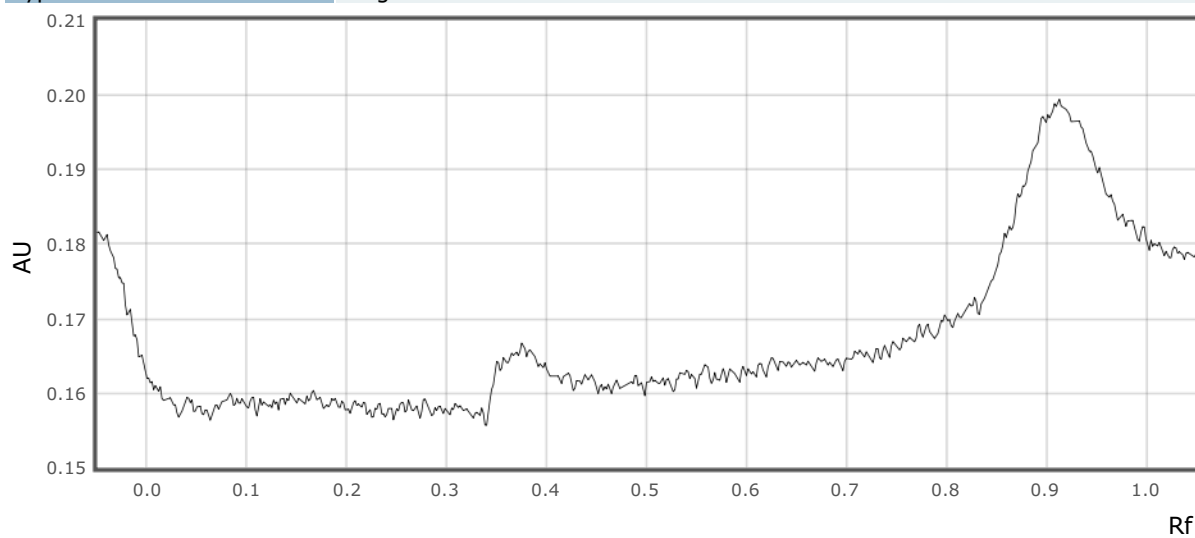


Track 8:

Type Single λ

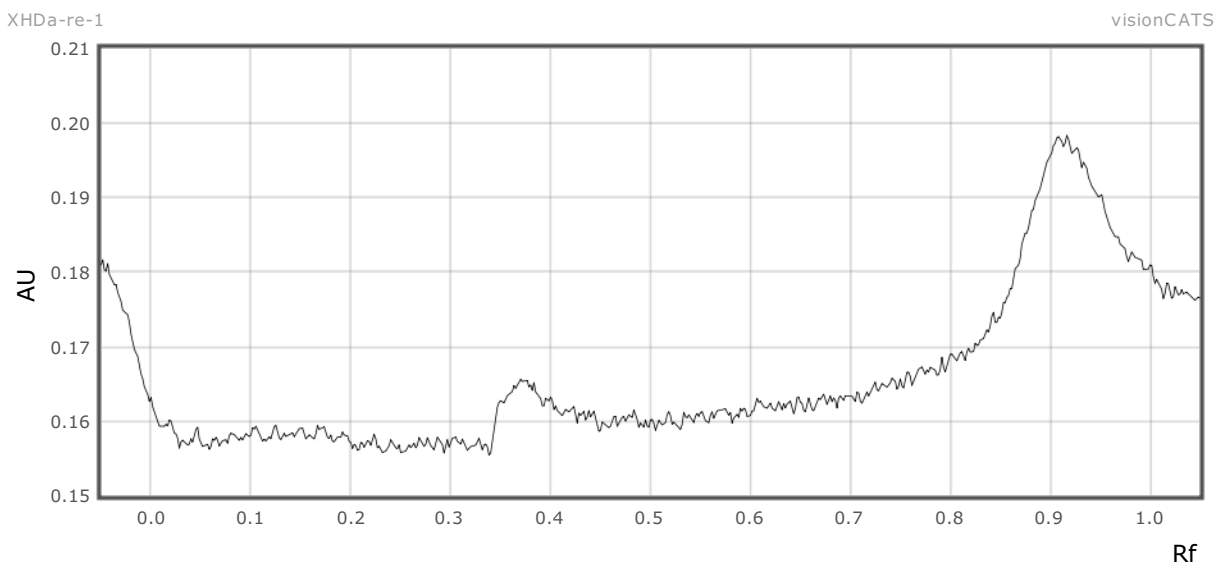


Track 9:

Type Single λ

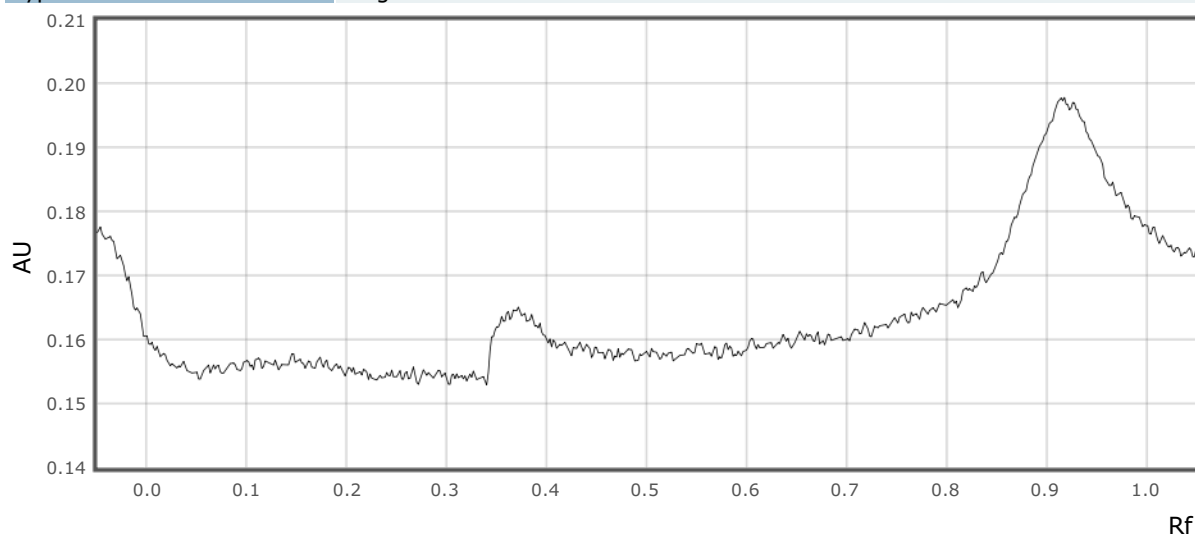


Track 10:

Type Single λ

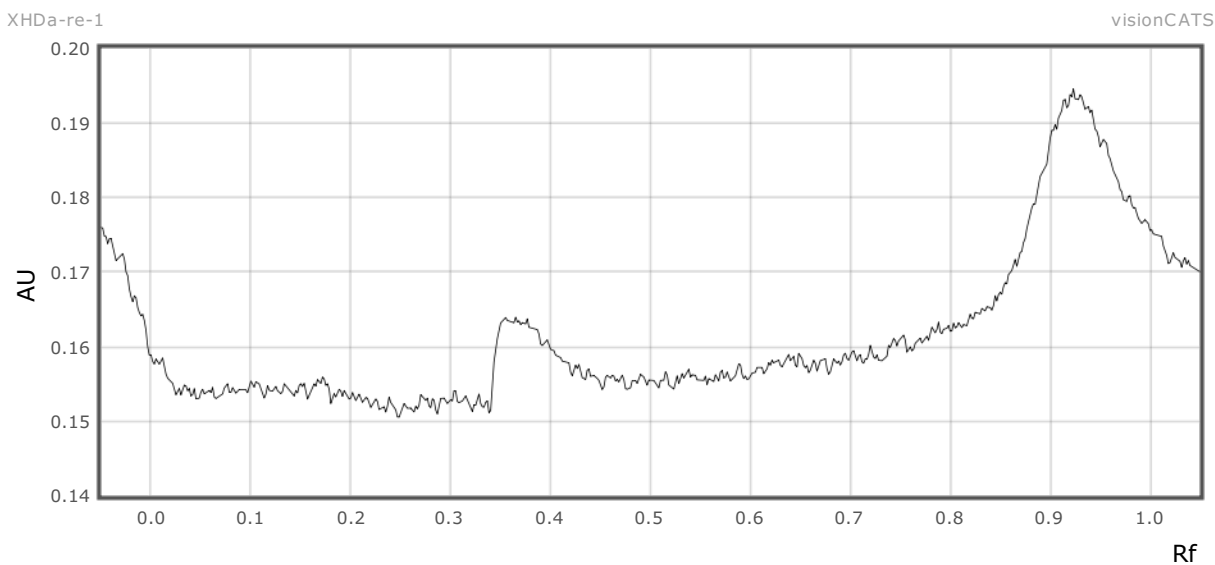

Track 11:

Type Single λ

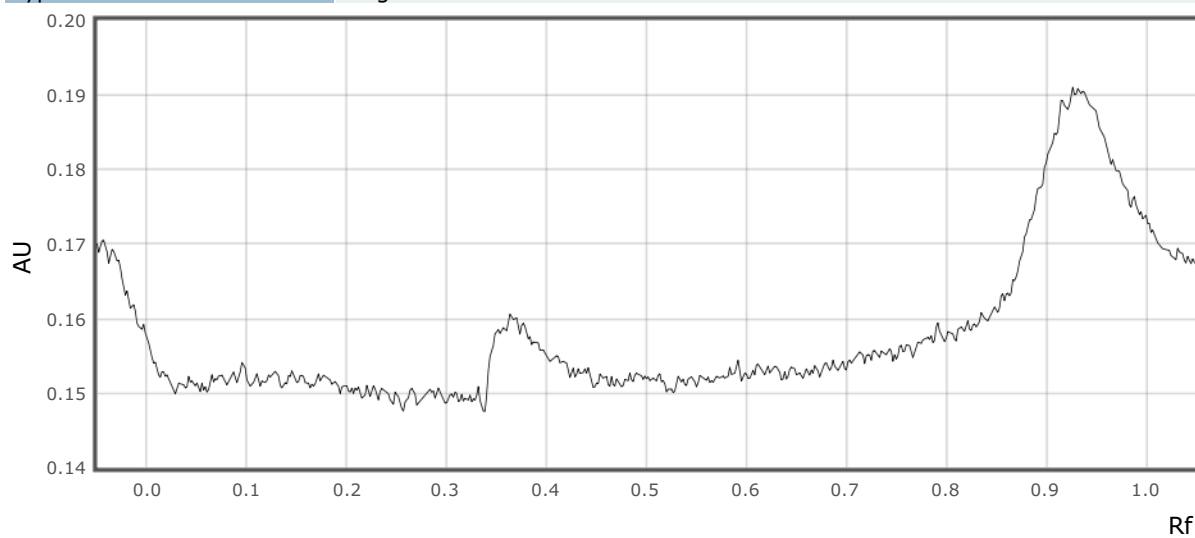


Track 12:

Type Single λ

XHDa-re-1


visionCATS

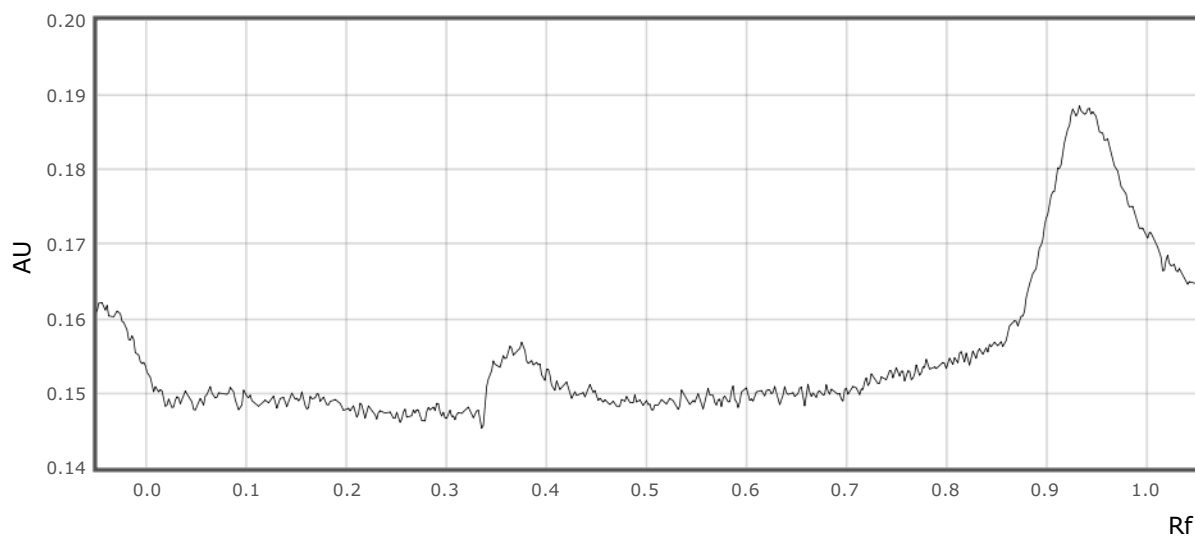

Track 13:

Type


Single λ

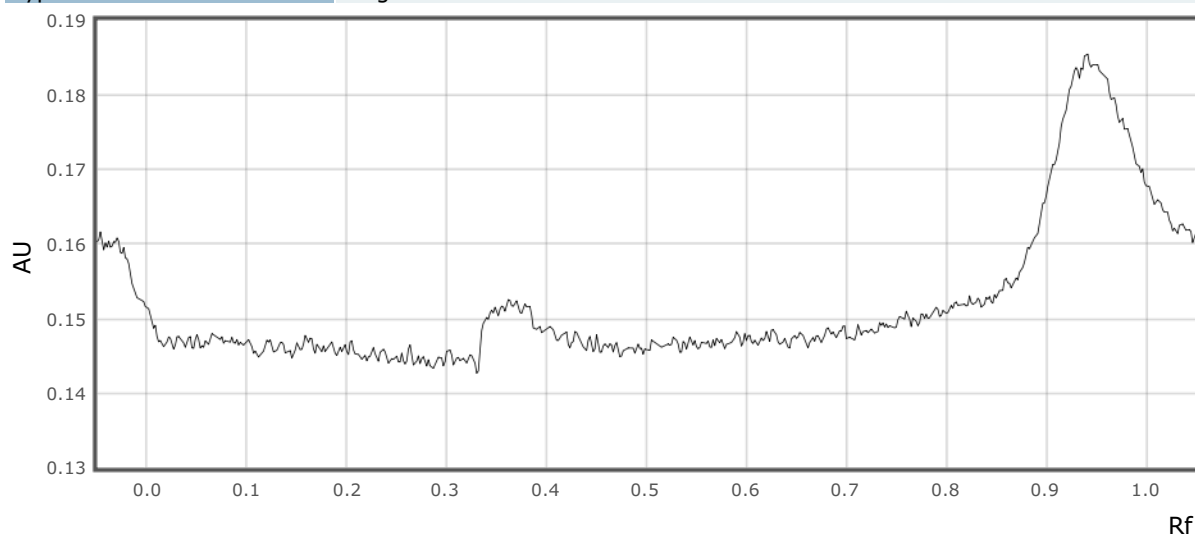

Track 14:

Type


Single λ

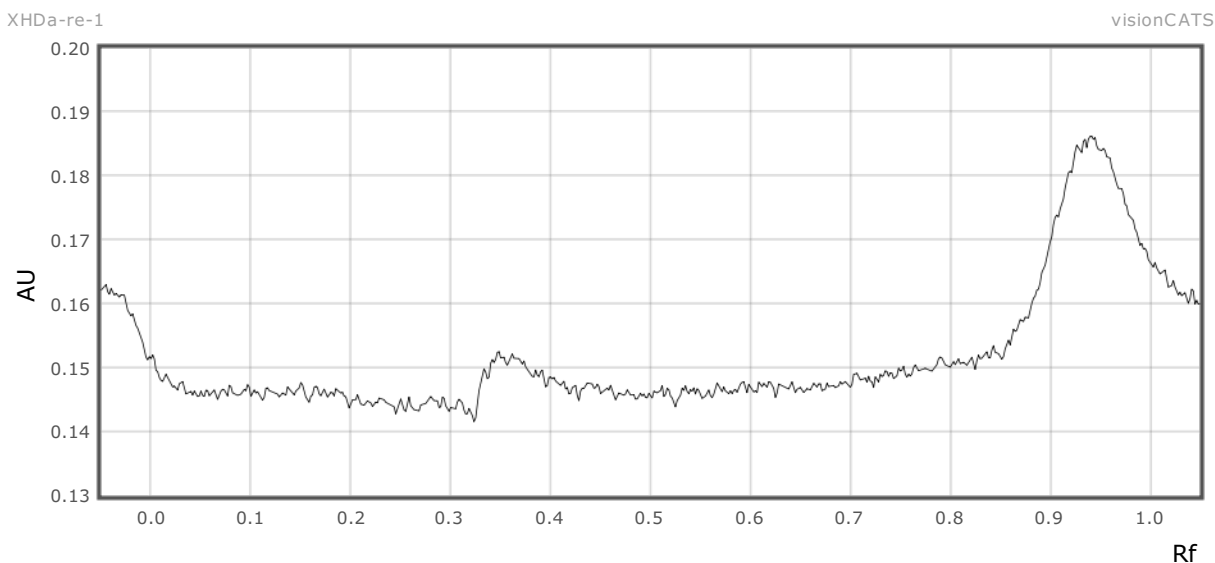

Track 15:

Type

Single λ

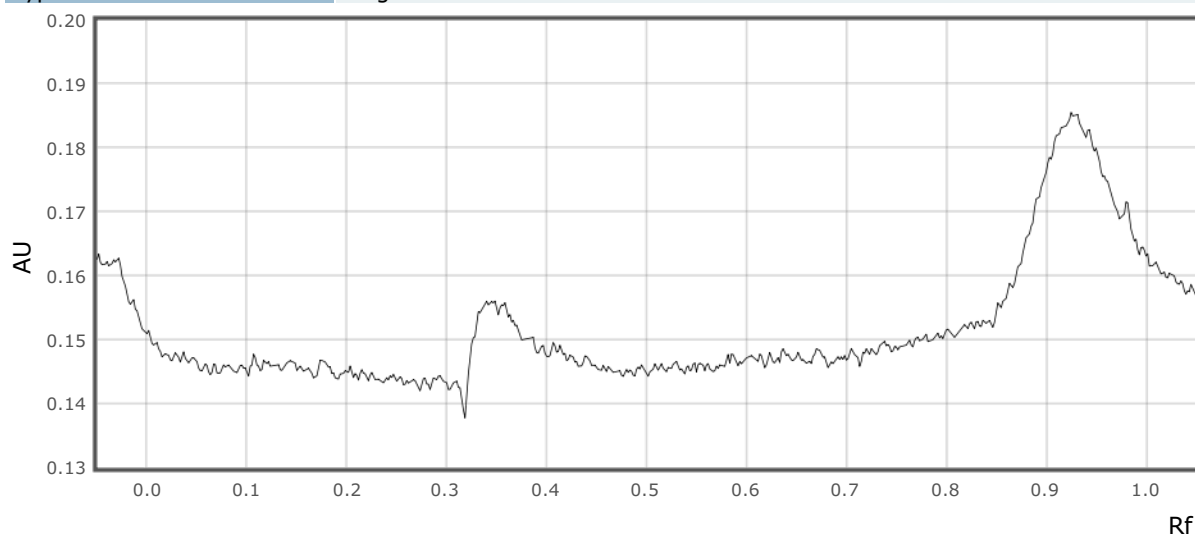

Derivatization 1 - dip:

Executed

07-Jun-2019 23:10:06 visionCATSuser


Take image derivatized plate 1a - Visualizer (S/N: 230515):

Executed

07-Jun-2019 23:13:01 visionCATSuser

XHDa-re-1
RT White


visionCATS
Derivatized, RemTransVis

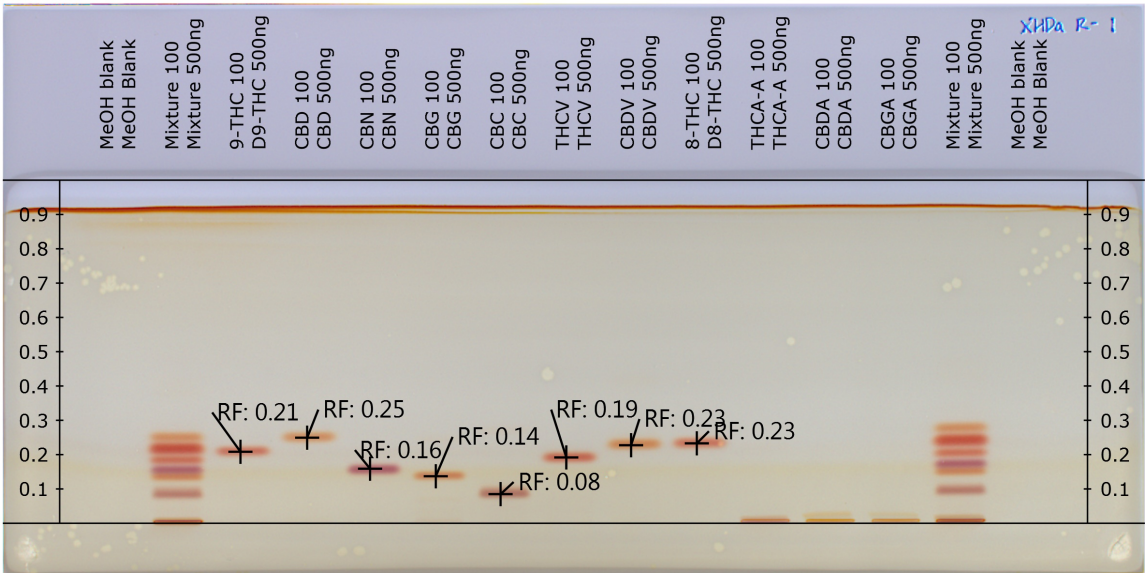

Exposure	0.068 s
Contrast	1
Normalized exposure	Disabled
Clarify	Disabled
White balance	1.16, 1.09, 0.82

R 366

Derivatized, Remission366

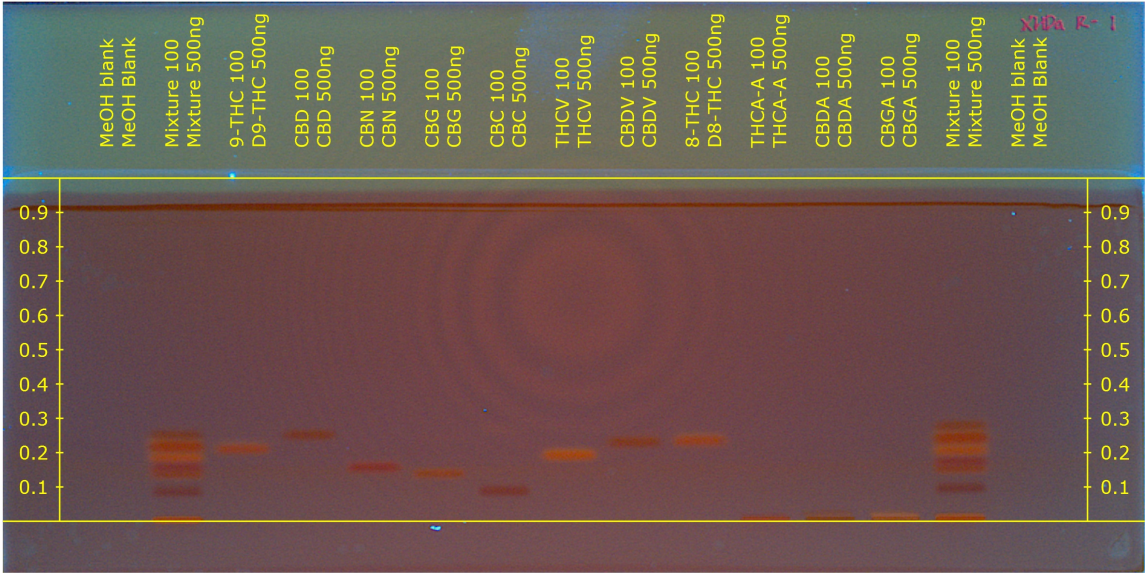

Exposure	9.999 s
Contrast	1
Normalized exposure	Disabled
Clarify	Disabled
White balance	1.00, 1.00, 1.00

Evaluation 1 :

XHDa-re-1

visionCATS

Validated	false
Step	Take image derivatized plate 1a
Concentration unit type	Mass / volume
Notes	

Definition:

References:

9-THC 100

Substance Name	Concentration	Purity
9-THC	100.000 µg/ml	100.00 %

CBD 100

Substance Name	Concentration	Purity
CBD	100.000 µg/ml	100.00 %

CBN 100

Substance Name	Concentration	Purity
CBN	100.000 µg/ml	100.00 %

CBG 100

Substance Name	Concentration	Purity
CBG	100.000 µg/ml	100.00 %

CBC 100

Substance Name	Concentration	Purity
CBC	100.000 µg/ml	100.00 %

THCV 100

Substance Name	Concentration	Purity
THCV	100.000 µg/ml	100.00 %

CBDV 100

Substance Name	Concentration	Purity
CBDV	100.000 µg/ml	100.00 %

8-THC 100

Substance Name	Concentration	Purity
8-THC	100.000 µg/ml	100.00 %

THCA-A 100

Substance Name	Concentration	Purity
THCA-A	100.000 µg/ml	100.00 %

CBDA 100

Substance Name	Concentration	Purity
CBDA	100.000 µg/ml	100.00 %

CBGA 100

Substance Name	Concentration	Purity
CBGA	100.000 µg/ml	100.00 %

XHDa-re-1

visionCATS

Samples:

Vial ID	Amount	Volume solution	Reference amount	Related to
MeOH blank		0.00 ml		
Mixture 100		0.00 ml		

Integration parameters:


Bounds	[0.000,1.000]
Smoothing	Savitzky-Golay of order 3 and window 7
Baseline correction	Lowest slope with noise 0.05
Profile subtraction	Profile subtraction from track 1
Peaks detection	Gauss (legacy) with sensitivity 0.1, separation 1 and threshold 0.1

Scan:

Wavelength	RT White
------------	----------

Track 1:


Type	Sample
Vial ID	MeOH blank
Description	MeOH Blank
Volume	2.0 µl

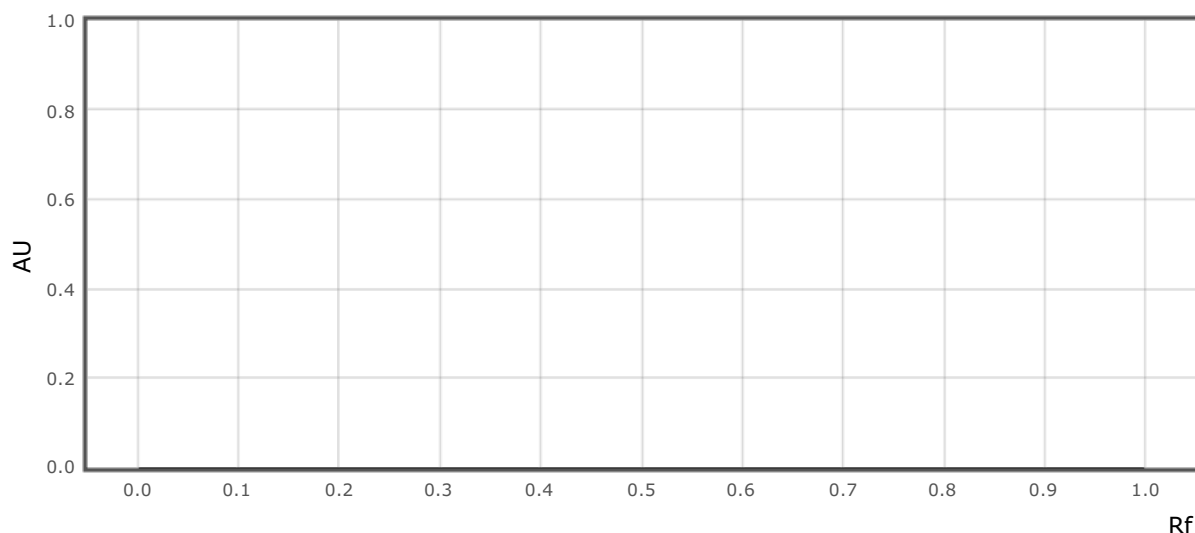

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		

Track 2:


Type	Sample
Vial ID	Mixture 100
Description	Mixture 500ng
Volume	5.0 µl

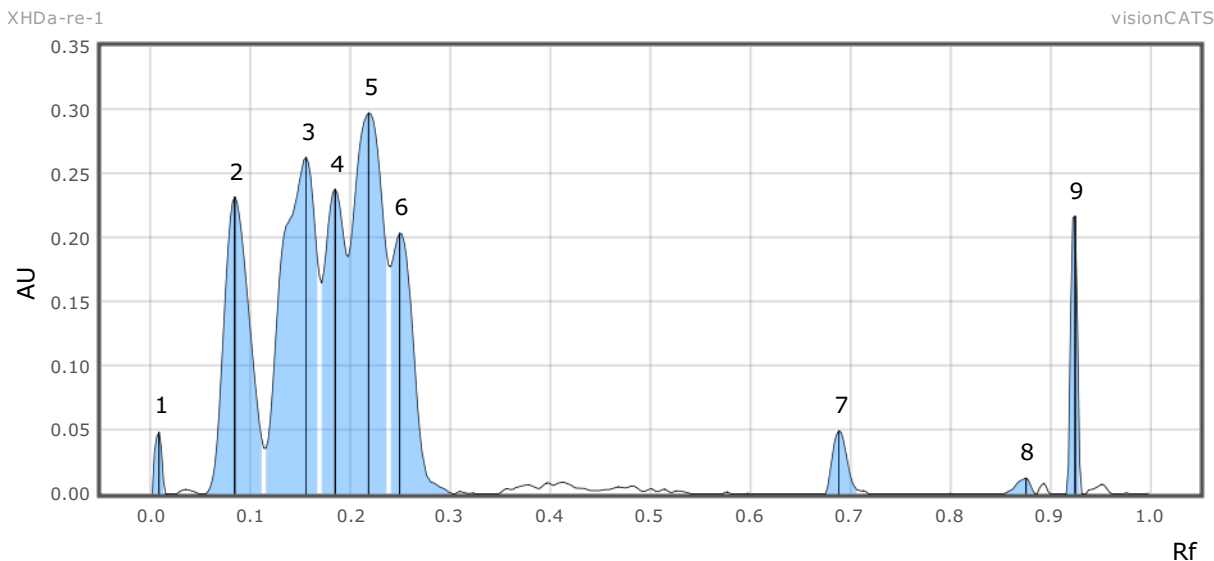

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.001	0.0000	0.008	0.0483	3.09	0.015	0.0000	0.00038	0.94	No	
2	0.055	0.0000	0.084	0.2321	14.86	0.113	0.0357	0.00681	16.73	No	
3	0.115	0.0355	0.155	0.2630	16.84	0.169	0.1697	0.01016	24.94	No	
4	0.171	0.1647	0.184	0.2380	15.24	0.198	0.1853	0.00559	13.73	No	
5	0.198	0.1853	0.218	0.2976	19.06	0.238	0.1783	0.01010	24.81	No	
6	0.240	0.1775	0.249	0.2037	13.04	0.303	0.0000	0.00497	12.20	No	
7	0.675	0.0000	0.689	0.0495	3.17	0.711	0.0023	0.00083	2.03	No	
8	0.854	0.0000	0.876	0.0124	0.79	0.885	0.0000	0.00019	0.48	No	
9	0.916	0.0000	0.925	0.2170	13.90	0.932	0.0000	0.00168	4.13	No	

Track 3:

Type	Reference
Vial ID	9-THC 100
Description	D9-THC 500ng
Volume	5.0 µl

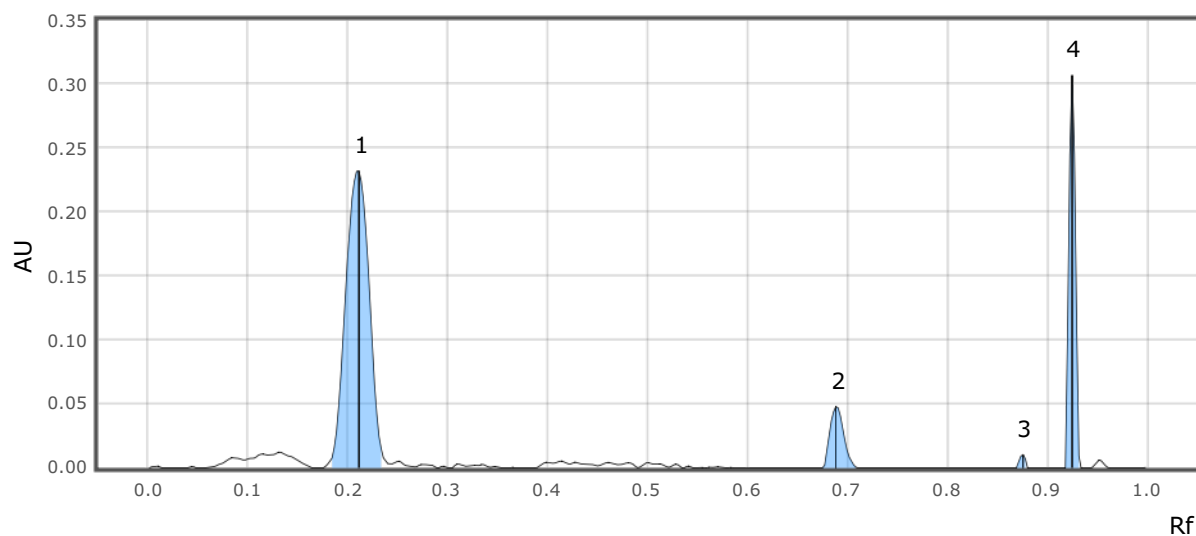


XHDa-re-1

visionCATS

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.184	0.0076	0.211	0.2319	38.86	0.235	0.0078	0.00628	66.84	Yes	9-THC
2	0.675	0.0000	0.689	0.0479	8.02	0.711	0.0000	0.00076	8.07	No	
3	0.869	0.0000	0.876	0.0103	1.73	0.880	0.0000	0.00007	0.73	No	
4	0.918	0.0000	0.925	0.3067	51.39	0.934	0.0000	0.00229	24.35	No	

Track 4:

Type	Reference
Vial ID	CBD 100
Description	CBD 500ng
Volume	5.0 µl

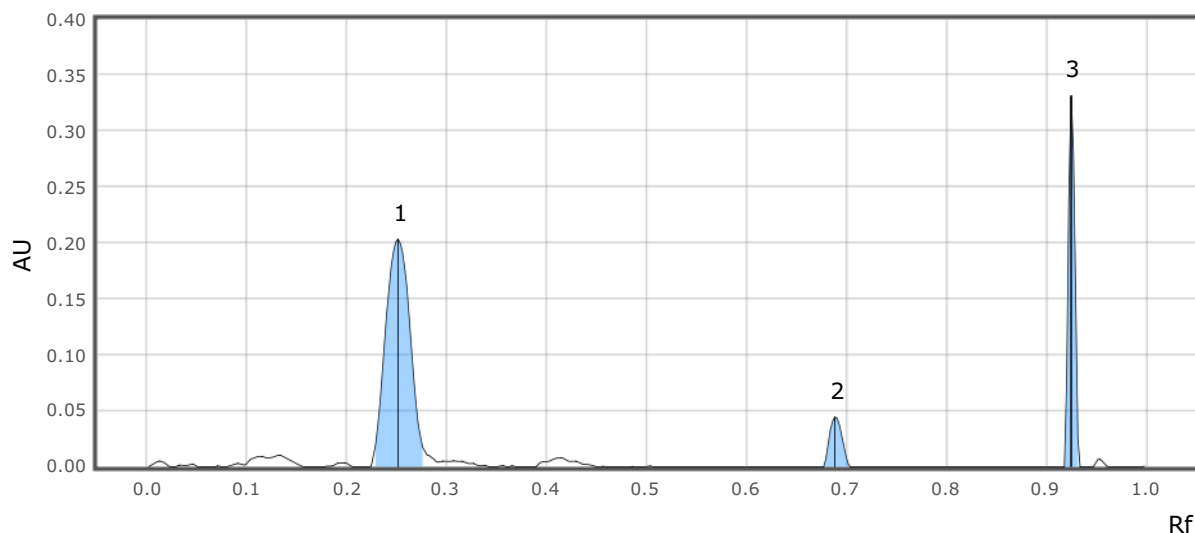


Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.228	0.0199	0.251	0.2034	35.11	0.276	0.0178	0.00571	64.83	Yes	CBD
2	0.677	0.0000	0.689	0.0444	7.67	0.704	0.0000	0.00064	7.26	No	
3	0.918	0.0000	0.925	0.3315	57.22	0.934	0.0000	0.00246	27.92	No	

Track 5:

Type	Reference
Vial ID	CBN 100
Description	CBN 500ng
Volume	5.0 µl

XHDa-re-1


visionCATS

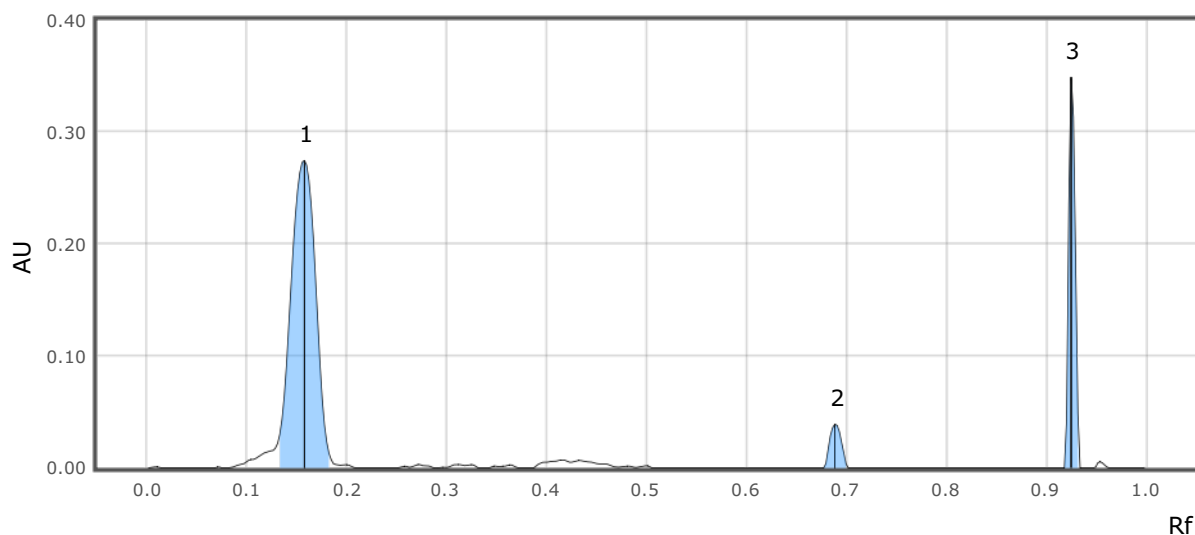

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.132	0.0218	0.158	0.2745	41.45	0.183	0.0130	0.00779	71.29	Yes	CBN
2	0.677	0.0000	0.689	0.0390	5.88	0.702	0.0000	0.00052	4.77	No	
3	0.918	0.0000	0.925	0.3488	52.66	0.934	0.0000	0.00261	23.94	No	

Track 6:

Type	Reference
Vial ID	CBG 100
Description	CBG 500ng
Volume	5.0 µl

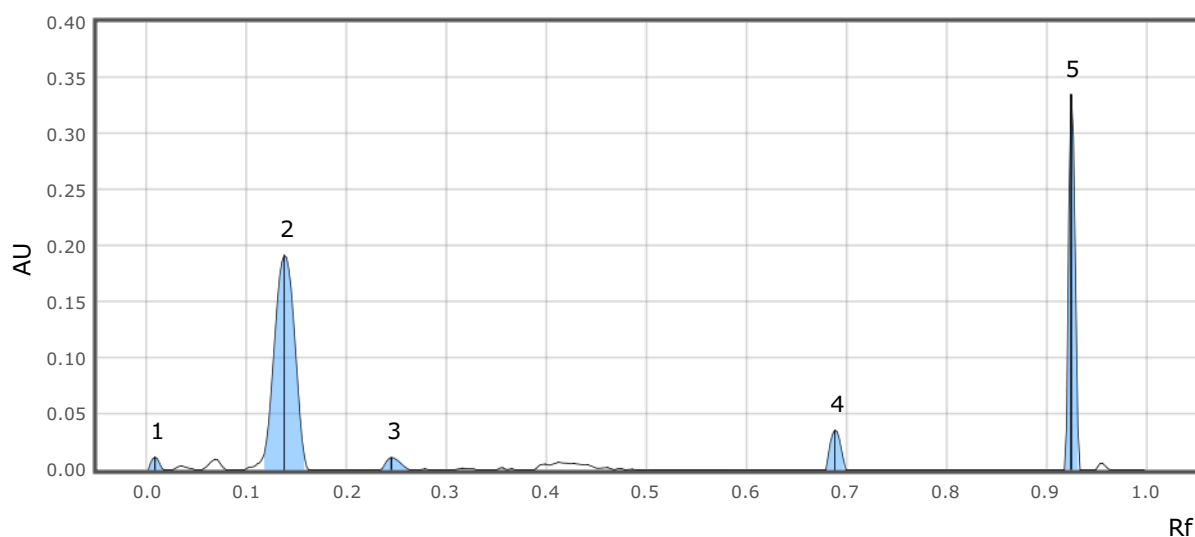


XHDa-re-1

visionCATS

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.001	0.0000	0.008	0.0112	1.91	0.017	0.0000	0.00010	1.32	No	
2	0.116	0.0095	0.137	0.1917	32.77	0.159	0.0027	0.00451	58.62	Yes	CBG
3	0.233	0.0000	0.245	0.0110	1.87	0.265	0.0000	0.00017	2.25	No	
4	0.680	0.0000	0.689	0.0356	6.09	0.700	0.0000	0.00043	5.56	No	
5	0.918	0.0000	0.925	0.3356	57.36	0.934	0.0000	0.00248	32.24	No	

Track 7:

Type	Reference
Vial ID	CBC 100
Description	CBC 500ng
Volume	5.0 µl

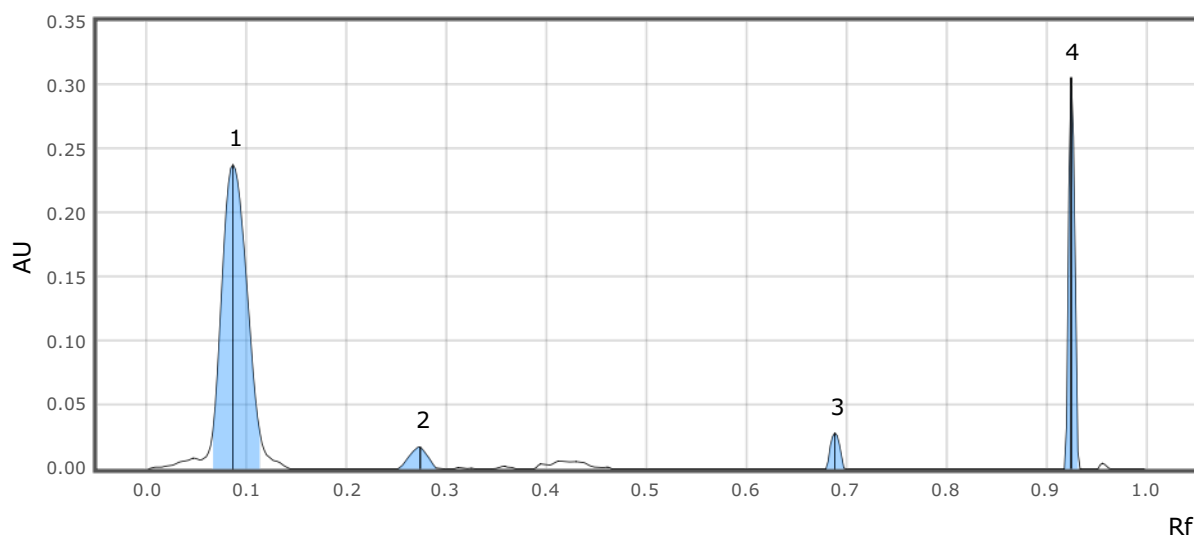


Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.065	0.0183	0.086	0.2377	40.39	0.114	0.0286	0.00687	71.05	Yes	CBC
2	0.251	0.0000	0.274	0.0169	2.87	0.291	0.0004	0.00035	3.62	No	
3	0.680	0.0000	0.689	0.0281	4.78	0.700	0.0000	0.00030	3.09	No	
4	0.918	0.0000	0.925	0.3058	51.96	0.934	0.0000	0.00215	22.24	No	

Track 8:

Type	Reference
Vial ID	THCV 100
Description	THCV 500ng
Volume	5.0 µl

XHDa-re-1


visionCATS

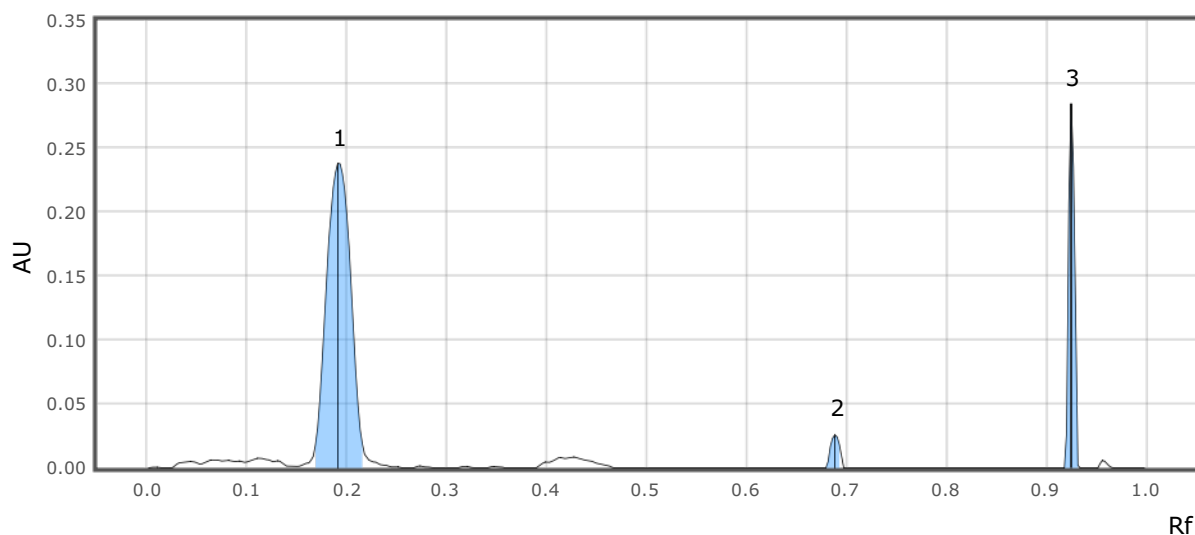

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.168	0.0179	0.191	0.2380	43.40	0.216	0.0188	0.00664	75.05	Yes	THCV
2	0.680	0.0000	0.689	0.0258	4.70	0.697	0.0000	0.00027	3.09	No	
3	0.918	0.0000	0.925	0.2846	51.90	0.934	0.0000	0.00194	21.87	No	

Track 9:

Type	Reference
Vial ID	CBDV 100
Description	CBDV 500ng
Volume	5.0 µl

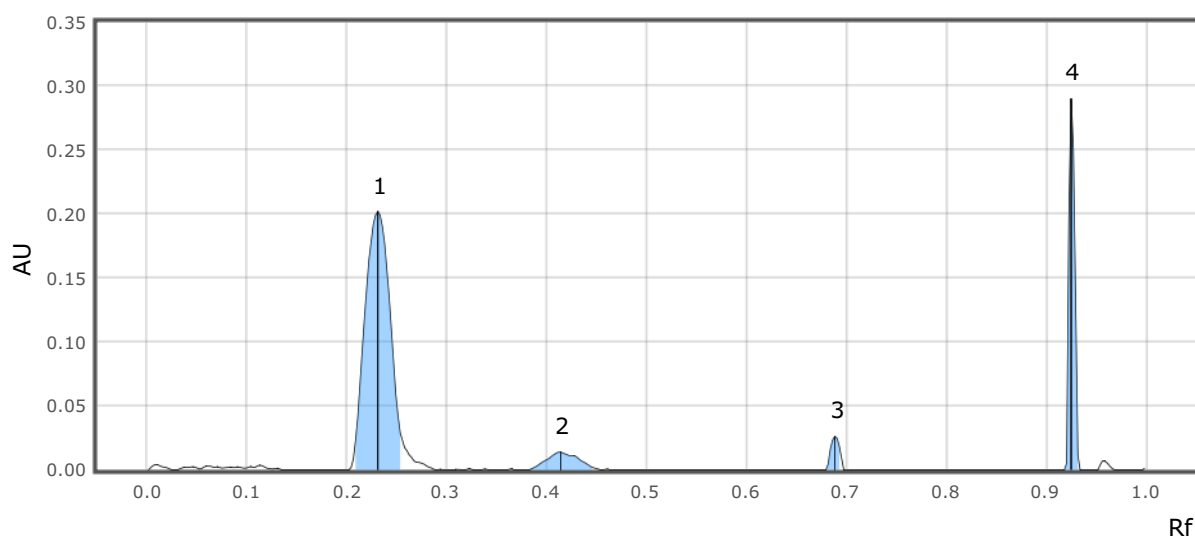


Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.207	0.0085	0.231	0.2019	37.95	0.255	0.0229	0.00584	68.02	Yes	CBDV
2	0.381	0.0000	0.414	0.0138	2.59	0.454	0.0000	0.00051	5.92	No	
3	0.680	0.0000	0.689	0.0263	4.94	0.697	0.0000	0.00027	3.19	No	
4	0.918	0.0000	0.925	0.2900	54.51	0.934	0.0000	0.00196	22.87	No	

XHDa-re-1


visionCATS

Track 10:	
Type	Reference
Vial ID	8-THC 100
Description	D8-THC 500ng
Volume	5.0 µl

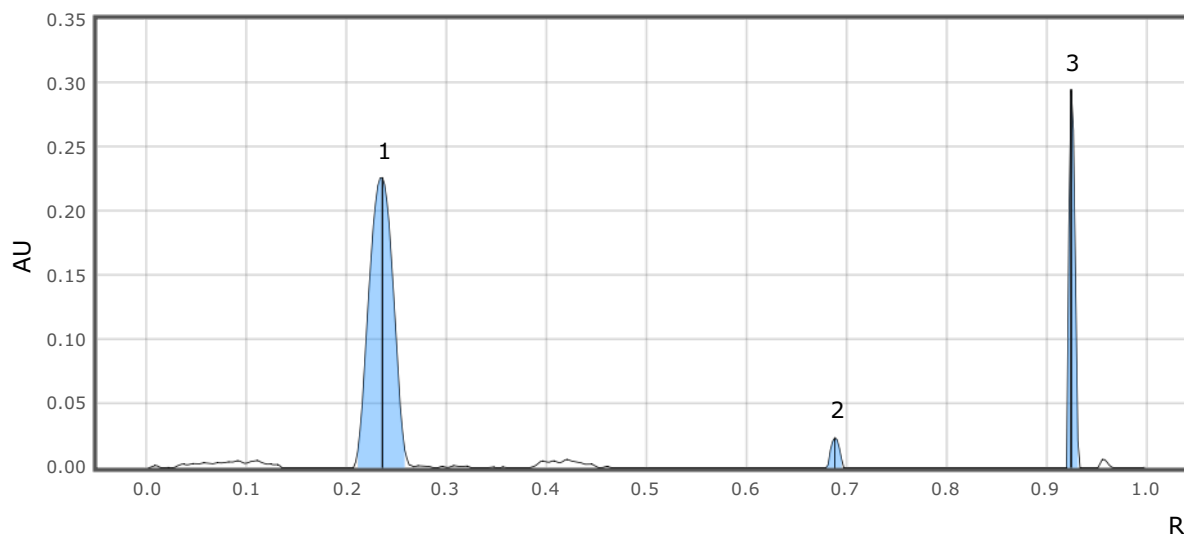

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.210	0.0130	0.236	0.2263	41.54	0.259	0.0138	0.00630	73.62	Yes	8-THC
2	0.680	0.0000	0.689	0.0235	4.31	0.697	0.0000	0.00023	2.70	No	
3	0.921	0.0000	0.925	0.2950	54.15	0.934	0.0000	0.00203	23.68	No	

Track 11:	
Type	Reference
Vial ID	THCA-A 100
Description	THCA-A 500ng
Volume	5.0 µl

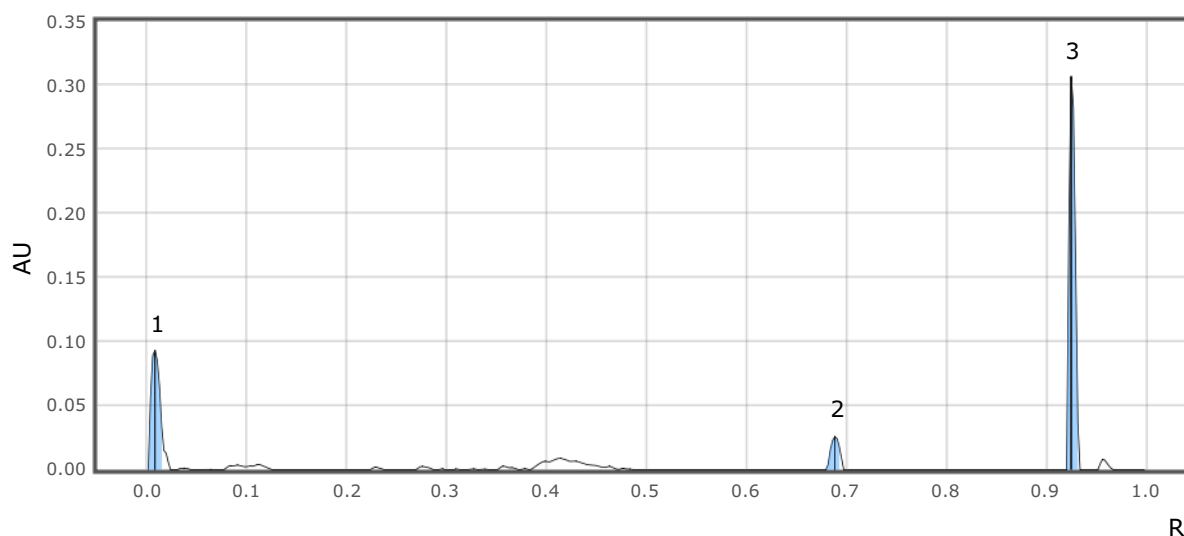


XHDa-re-1

visionCATS

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.001	0.0000	0.008	0.0932	21.89	0.017	0.0150	0.00096	28.15	Yes	THCA-A
2	0.680	0.0000	0.689	0.0259	6.07	0.697	0.0000	0.00027	7.80	No	
3	0.921	0.0000	0.925	0.3068	72.04	0.934	0.0000	0.00218	64.04	No	

Track 12:


Type	Reference
Vial ID	CBDA 100
Description	CBDA 500ng
Volume	5.0 µl

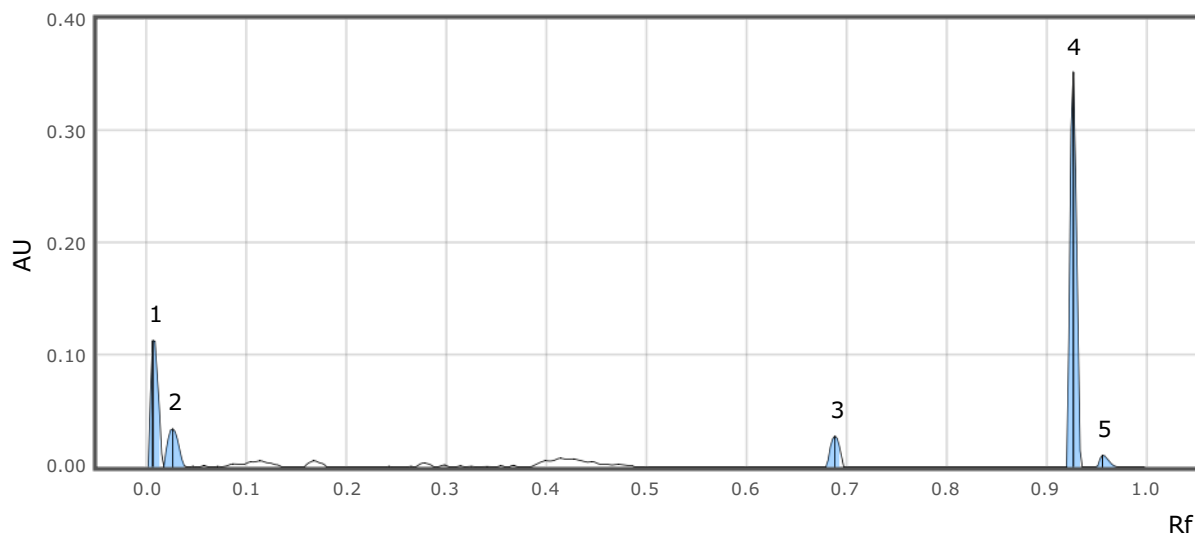

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.001	0.0000	0.006	0.1128	20.99	0.015	0.0116	0.00095	21.84	Yes	CBDA
2	0.017	0.0000	0.026	0.0339	6.30	0.039	0.0000	0.00042	9.53	No	
3	0.680	0.0000	0.689	0.0277	5.15	0.697	0.0000	0.00029	6.58	No	
4	0.921	0.0000	0.927	0.3527	65.66	0.936	0.0000	0.00261	59.75	No	
5	0.950	0.0000	0.956	0.0102	1.90	0.972	0.0000	0.00010	2.30	No	

Track 13:


Type	Reference
Vial ID	CBGA 100
Description	CBGA 500ng
Volume	5.0 µl

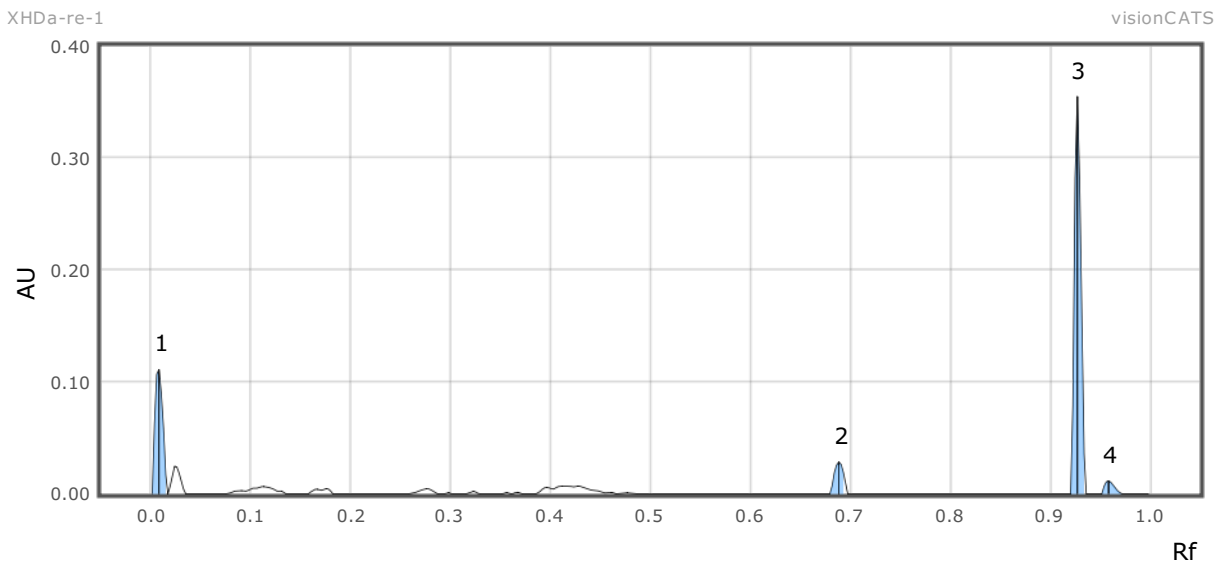

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.001	0.0000	0.008	0.1110	21.94	0.015	0.0169	0.00098	24.15	Yes	CBGA
2	0.680	0.0000	0.689	0.0284	5.62	0.697	0.0000	0.00030	7.46	No	
3	0.921	0.0000	0.927	0.3549	70.16	0.936	0.0000	0.00264	65.29	No	
4	0.952	0.0000	0.959	0.0115	2.28	0.974	0.0000	0.00013	3.11	No	

Track 14:

Type	Sample
Vial ID	Mixture 100
Description	Mixture 500ng
Volume	5.0 µl

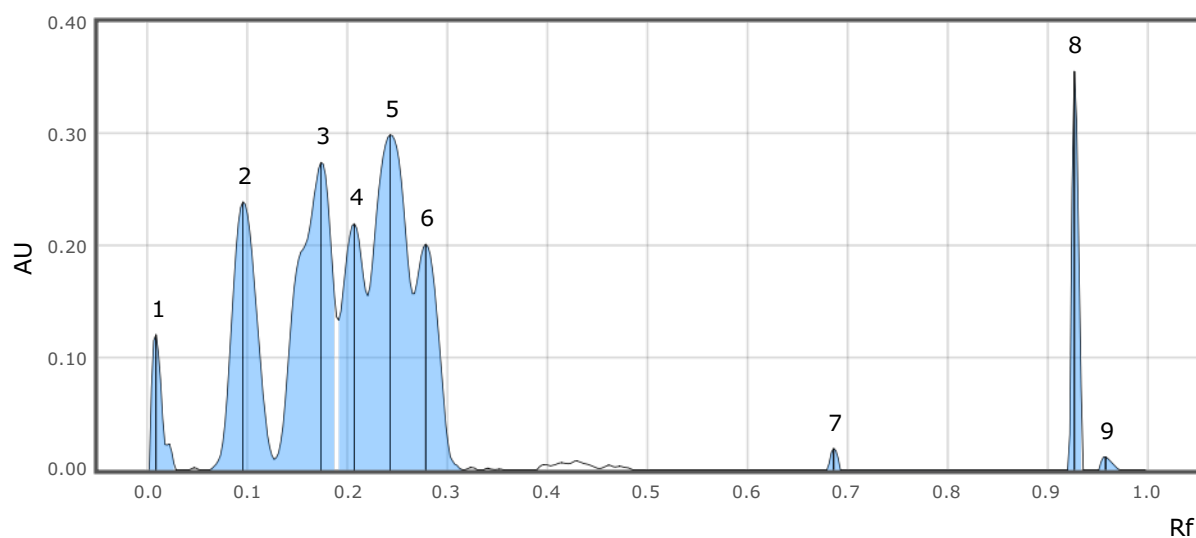


XHDa-re-1

visionCATS

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.001	0.0000	0.008	0.1208	6.93	0.028	0.0000	0.00141	3.25	No	
2	0.062	0.0000	0.095	0.2394	13.74	0.126	0.0093	0.00676	15.64	No	
3	0.126	0.0093	0.173	0.2746	15.77	0.189	0.1366	0.01052	24.34	No	
4	0.191	0.1336	0.207	0.2199	12.62	0.220	0.1555	0.00538	12.44	No	
5	0.220	0.1555	0.242	0.2991	17.17	0.265	0.1572	0.01079	24.96	No	
6	0.265	0.1572	0.278	0.2016	11.57	0.316	0.0000	0.00536	12.41	No	
7	0.680	0.0000	0.686	0.0190	1.09	0.695	0.0000	0.00015	0.35	No	
8	0.921	0.0000	0.927	0.3560	20.44	0.936	0.0000	0.00272	6.30	No	
9	0.952	0.0000	0.959	0.0116	0.67	0.974	0.0000	0.00013	0.31	No	

Track 15:


Type	Sample
Vial ID	MeOH blank
Description	MeOH Blank
Volume	2.0 µl

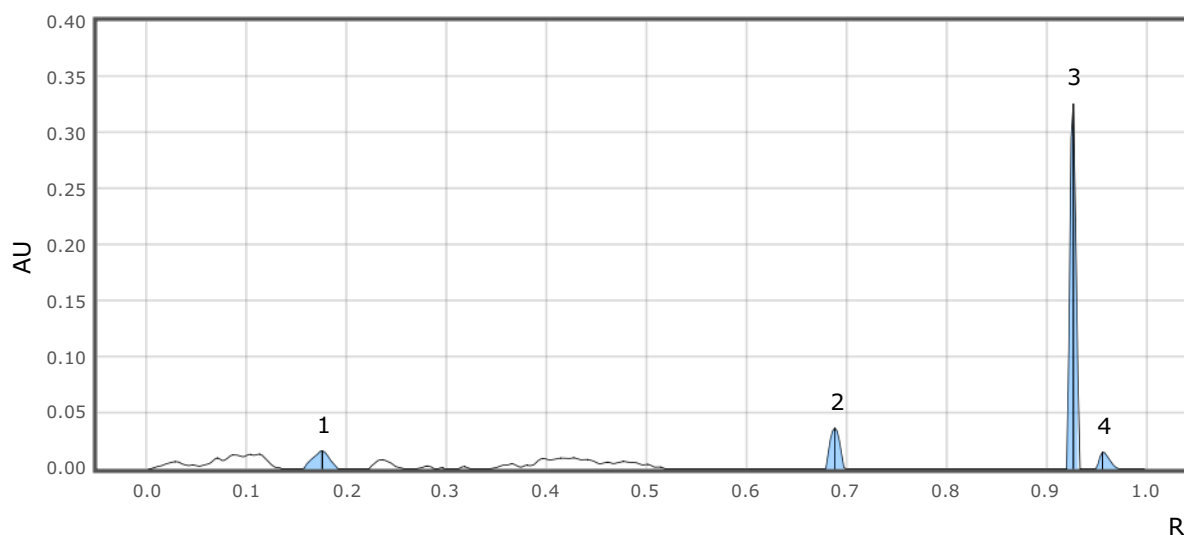

Peak #	Start		Max			End		Area		Manual peak	Substance Name
	Rf	H	Rf	H	%	Rf	H	A	%		
1	0.155	0.0000	0.175	0.0162	4.12	0.193	0.0000	0.00031	9.63	No	
2	0.677	0.0000	0.689	0.0365	9.27	0.700	0.0000	0.00041	12.90	No	
3	0.921	0.0000	0.927	0.3259	82.89	0.934	0.0000	0.00230	72.23	No	
4	0.950	0.0000	0.956	0.0146	3.72	0.974	0.0000	0.00017	5.24	No	


Calibration results:

Height calibration for substance 8-THC @ RT White:

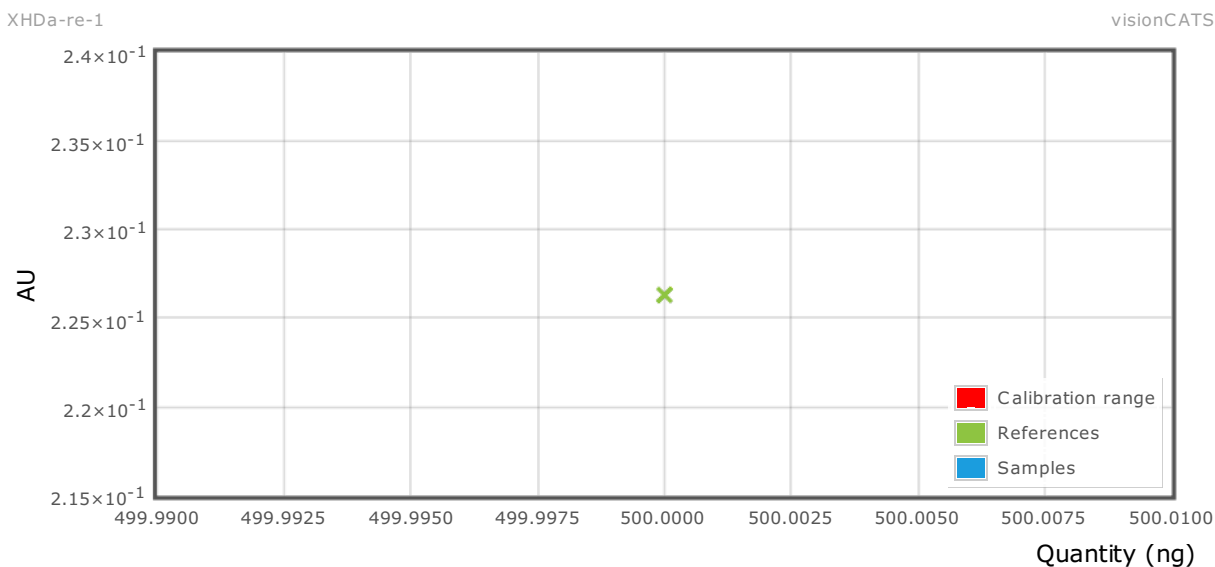

Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance 9-THC @ RT White:

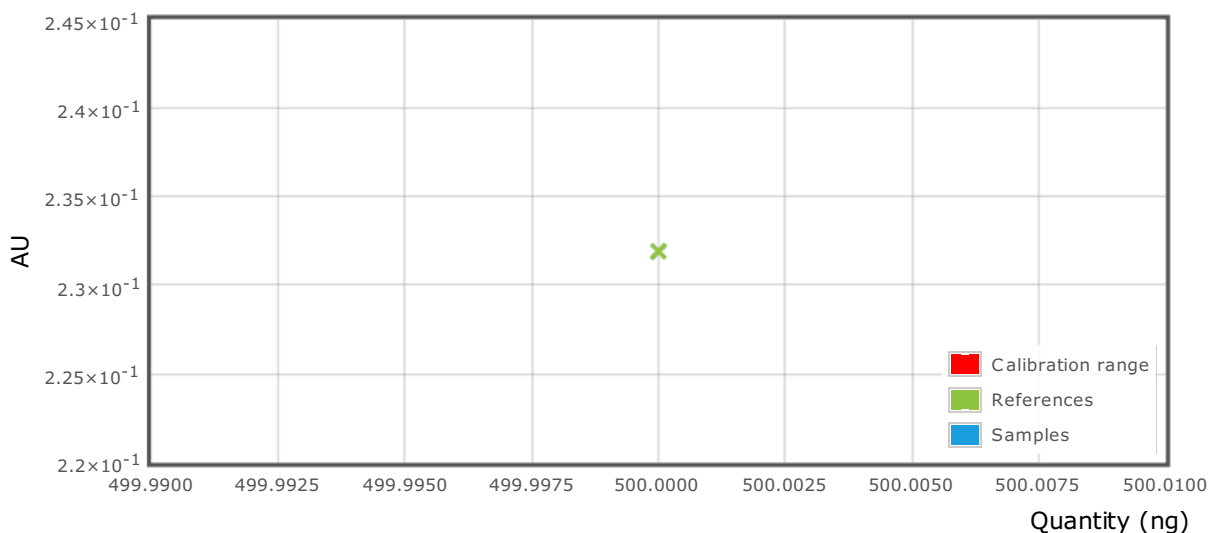


XHDa-re-1

visionCATS


Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance CBC @ RT White:

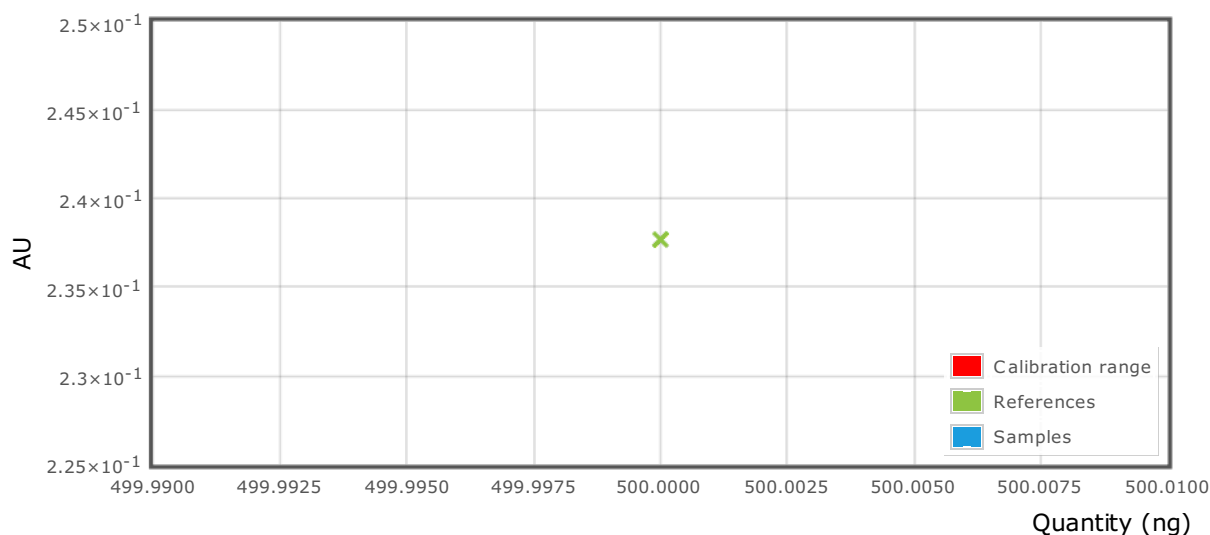


Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance CBD @ RT White:

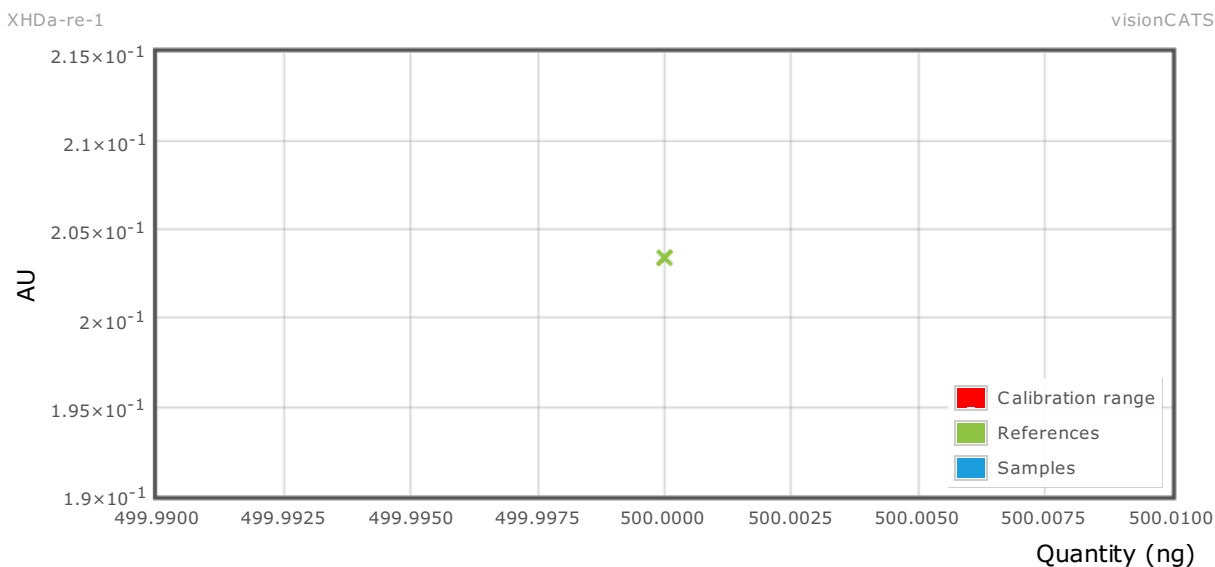

Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance CBDA @ RT White:

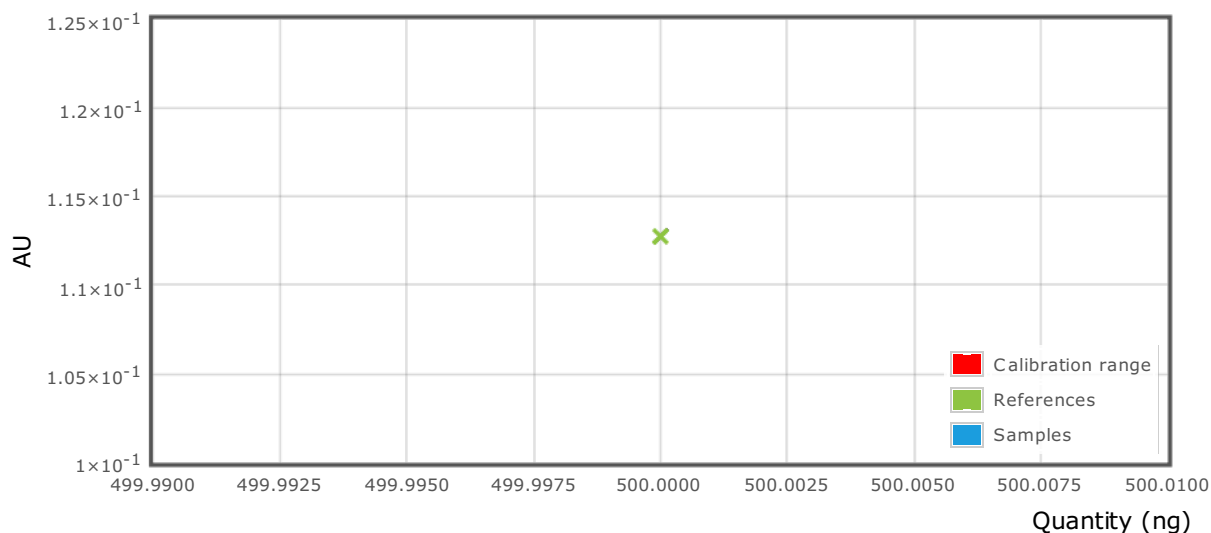


XHDa-re-1

visionCATS


Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance CBDV @ RT White:

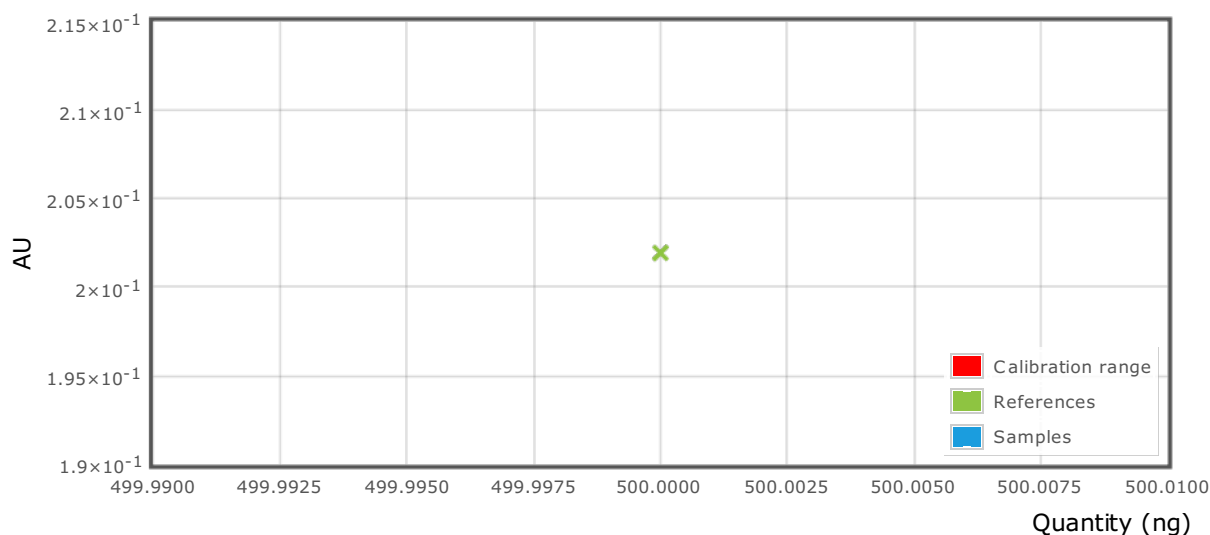


Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance CBG @ RT White:

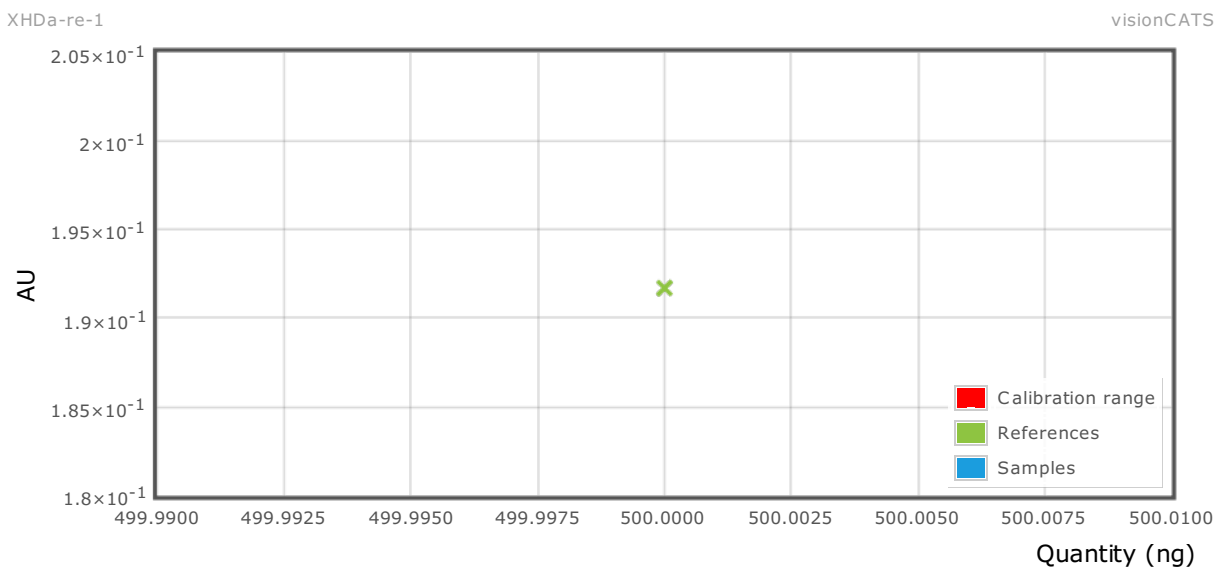

Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance CBGA @ RT White:

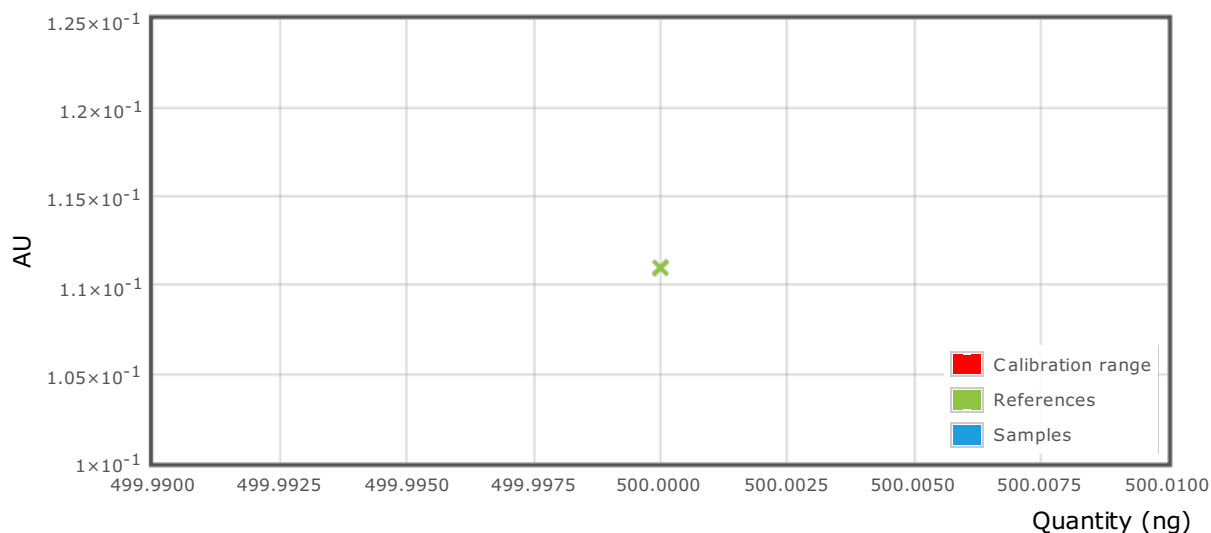


XHDa-re-1

visionCATS


Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance CBN @ RT White:

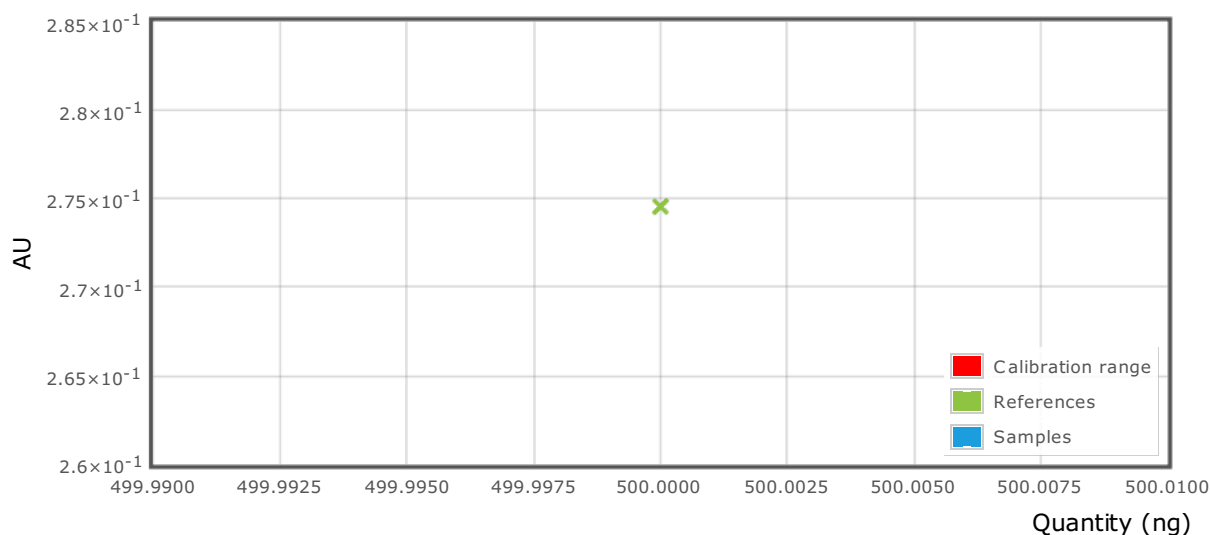


Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance THCA-A @ RT White:

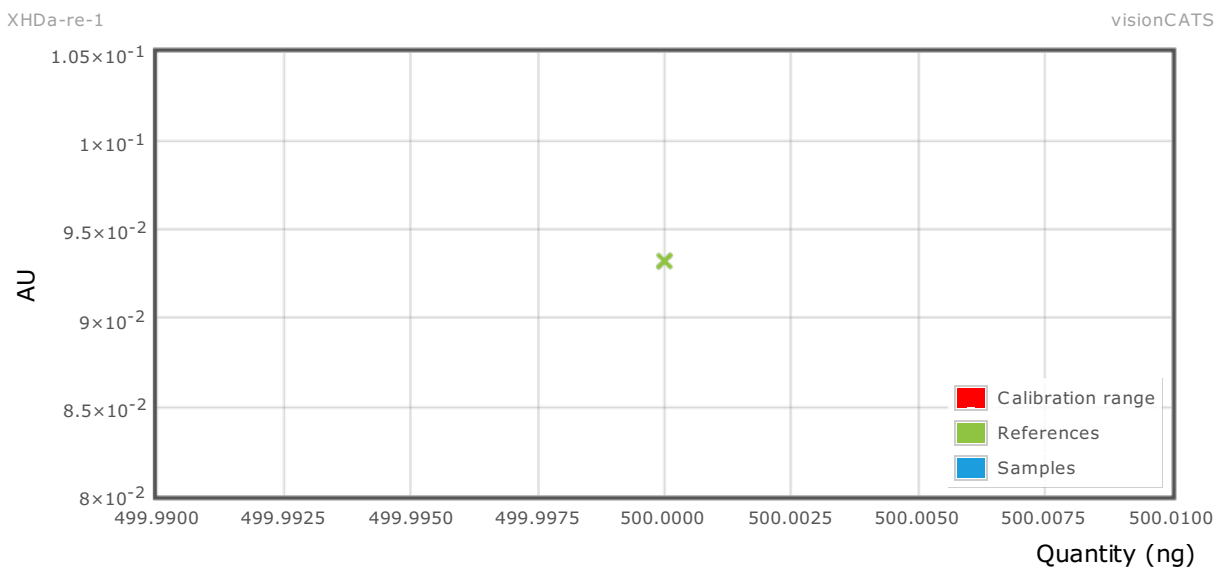

Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Height calibration for substance THCV @ RT White:

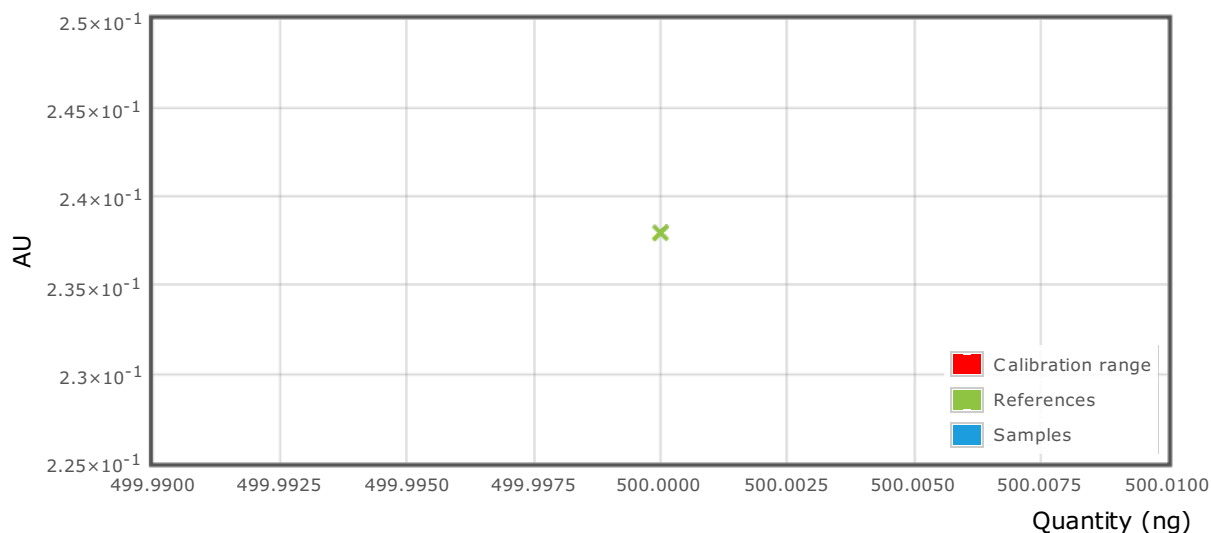

XHDa-re-1

visionCATS

Regression mode	Linear-2
Range deviation	5.00 %
Related substances	Default
Number of references	1
Calibration function	$y=0x$
Coefficient of variation	CV 0.00 %
Correlation coefficient	n/a
	Unable to compute the results for this substance because there wasn't enough groups of references replicas (at least 1 for Linear-1, 2 for Linear2 and Mime-1 and 3 for Polynomial and MiMe-2)

Results:

Substance having no available results		
	CBN	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	CBD	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	CBC	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	THCA-A	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	8-THC	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	CBGA	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	9-THC	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	CBDV	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	CBDA	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	CBG	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.
	THCV	There wasn't any sample application available in the assignments for this substance. Please check that the peaks were correctly detected and assigned for this substance.

A track marked with  means: this result is outside the regression range given by the reference assignments, but is included in the results because it is in the allowed range deviation.

Analyst:

Reviewer: